


Medical electrical equipment - Part 2-30: Particular requirements for the basic safety
and essential performance of automated non-invasive sphygmomanometers

CORRIGENDUM 1

Figure 201.101 – CUFF pressure PROTECTION DEVICE, triggered by overpressure in SINGLE FAULT CONDITION

Replace the existing figure with the following new figure:

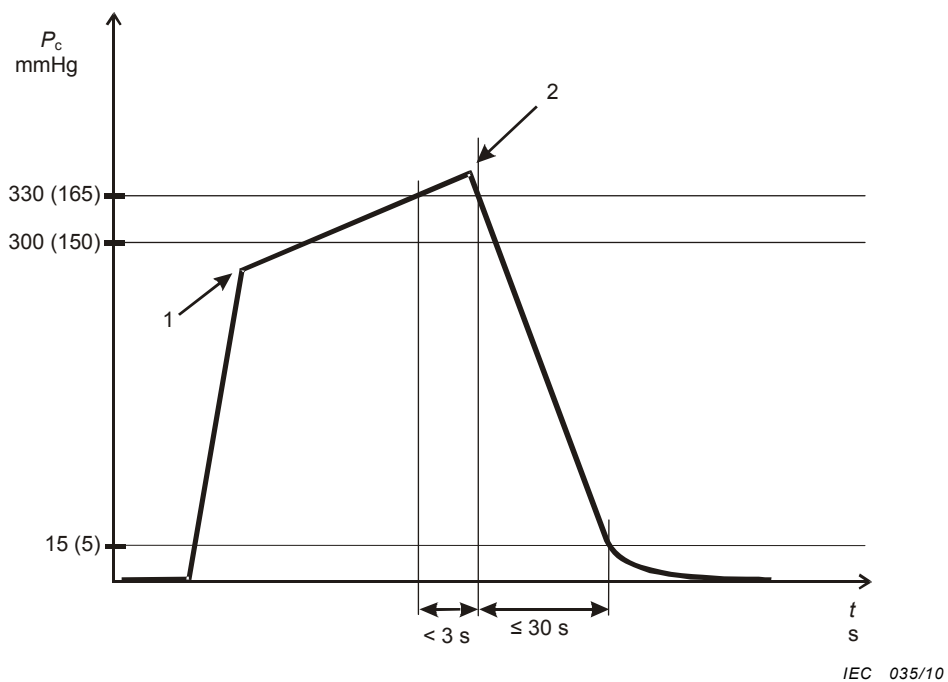

201.105.1 LONG-TERM AUTOMATIC MODE

In item a), delete “either” at the end of the first line and replace “or” with “and” at the end of the first dash.

201.105.3.2 NORMAL CONDITION

Delete “either” at the end of the first line and replace “or” with “and” at the end of the first dash.


CEI 80601-2-30
(Première édition – 2009)

Appareils électromédicaux –
Partie 2-30: Exigences particulières pour la sécurité de base et les performances
essentielles des sphygmomanomètres non invasifs automatiques

CORRIGENDUM 1

Figure 201.101

Remplacer la figure existante par la nouvelle figure suivante ;

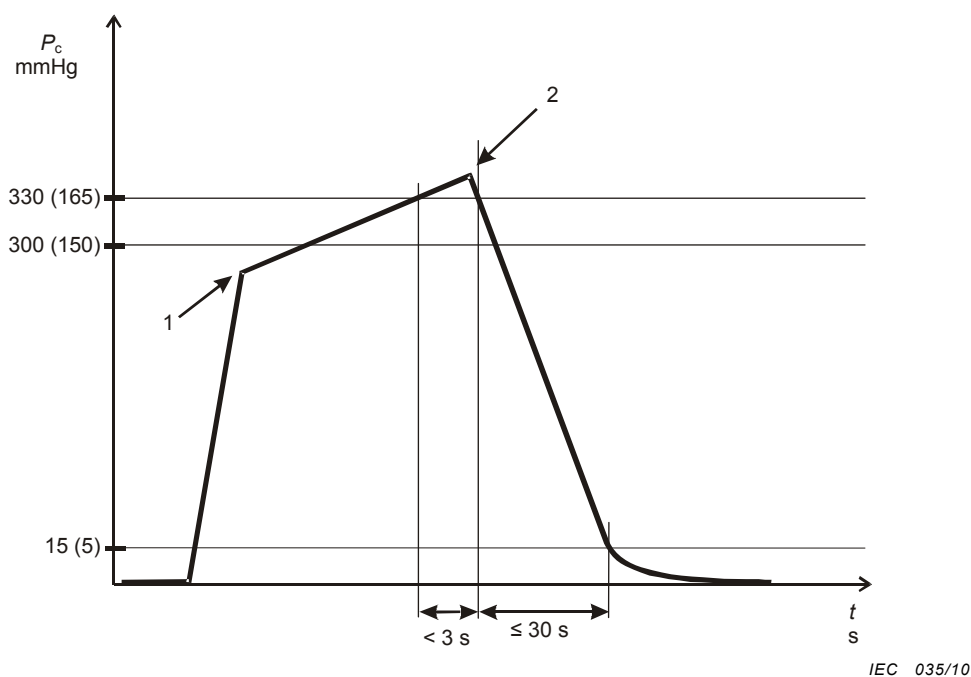

201.105.1 MODE AUTOMATIQUE LONGUE DURÉE

Dans l'item a), remplacer « ou » par « et » à la fin du premier tiret.

201.105.3.2 CONDITION NORMALE

Supprimer « soit » à la fin de la première ligne et remplacer « ou » par « et » à la fin du premier tiret.