

INTERNATIONAL STANDARD

NORME INTERNATIONALE

Electrical equipment for measurement, control and laboratory use – EMC requirements –

Part 3-2: Immunity requirements for safety-related systems and for equipment intended to perform safety-related functions (functional safety) – Industrial applications with specified electromagnetic environment

Matériel électrique de mesure, de commande et de laboratoire – Exigences relatives à la CEM –

Partie 3-2: Exigences d'immunité pour les systèmes relatifs à la sécurité et pour les matériels destinés à réaliser des fonctions relatives à la sécurité (sécurité fonctionnelle) – Applications industrielles dont l'environnement électromagnétique est spécifié



THIS PUBLICATION IS COPYRIGHT PROTECTED

Copyright © 2008 IEC, Geneva, Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester.

If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

Droits de reproduction réservés. Sauf indication contraire, aucune partie de cette publication ne peut être reproduite ni utilisée sous quelque forme que ce soit et par aucun procédé, électronique ou mécanique, y compris la photocopie et les microfilms, sans l'accord écrit de la CEI ou du Comité national de la CEI du pays du demandeur.

Si vous avez des questions sur le copyright de la CEI ou si vous désirez obtenir des droits supplémentaires sur cette publication, utilisez les coordonnées ci-après ou contactez le Comité national de la CEI de votre pays de résidence.

IEC Central Office
3, rue de Varembe
CH-1211 Geneva 20
Switzerland
Email: inmail@iec.ch
Web: www.iec.ch

About the IEC

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigenda or an amendment might have been published.

- Catalogue of IEC publications: www.iec.ch/searchpub

The IEC on-line Catalogue enables you to search by a variety of criteria (reference number, text, technical committee,...). It also gives information on projects, withdrawn and replaced publications.

- IEC Just Published: www.iec.ch/online_news/justpub

Stay up to date on all new IEC publications. Just Published details twice a month all new publications released. Available on-line and also by email.

- Electropedia: www.electropedia.org

The world's leading online dictionary of electronic and electrical terms containing more than 20 000 terms and definitions in English and French, with equivalent terms in additional languages. Also known as the International Electrotechnical Vocabulary online.

- Customer Service Centre: www.iec.ch/webstore/custserv

If you wish to give us your feedback on this publication or need further assistance, please visit the Customer Service Centre FAQ or contact us:

Email: csc@iec.ch

Tel.: +41 22 919 02 11

Fax: +41 22 919 03 00

A propos de la CEI

La Commission Electrotechnique Internationale (CEI) est la première organisation mondiale qui élabore et publie des normes internationales pour tout ce qui a trait à l'électricité, à l'électronique et aux technologies apparentées.

A propos des publications CEI

Le contenu technique des publications de la CEI est constamment revu. Veuillez vous assurer que vous possédez l'édition la plus récente, un corrigendum ou amendement peut avoir été publié.

- Catalogue des publications de la CEI: www.iec.ch/searchpub/cur_fut-f.htm

Le Catalogue en-ligne de la CEI vous permet d'effectuer des recherches en utilisant différents critères (numéro de référence, texte, comité d'études,...). Il donne aussi des informations sur les projets et les publications retirées ou remplacées.

- Just Published CEI: www.iec.ch/online_news/justpub

Restez informé sur les nouvelles publications de la CEI. Just Published détaille deux fois par mois les nouvelles publications parues. Disponible en-ligne et aussi par email.

- Electropedia: www.electropedia.org

Le premier dictionnaire en ligne au monde de termes électroniques et électriques. Il contient plus de 20 000 termes et définitions en anglais et en français, ainsi que les termes équivalents dans les langues additionnelles. Egalement appelé Vocabulaire Electrotechnique International en ligne.

- Service Clients: www.iec.ch/webstore/custserv/custserv_entry-f.htm

Si vous désirez nous donner des commentaires sur cette publication ou si vous avez des questions, visitez le FAQ du Service clients ou contactez-nous:

Email: csc@iec.ch

Tél.: +41 22 919 02 11

Fax: +41 22 919 03 00

INTERNATIONAL STANDARD

NORME INTERNATIONALE

Electrical equipment for measurement, control and laboratory use – EMC requirements –

Part 3-2: Immunity requirements for safety-related systems and for equipment intended to perform safety-related functions (functional safety) – Industrial applications with specified electromagnetic environment

Matériel électrique de mesure, de commande et de laboratoire – Exigences relatives à la CEM –

Partie 3-2: Exigences d'immunité pour les systèmes relatifs à la sécurité et pour les matériels destinés à réaliser des fonctions relatives à la sécurité (sécurité fonctionnelle) – Applications industrielles dont l'environnement électromagnétique est spécifié

INTERNATIONAL
ELECTROTECHNICAL
COMMISSION

COMMISSION
ELECTROTECHNIQUE
INTERNATIONALE

PRICE CODE
CODE PRIX

CONTENTS

FOREWORD.....	4
INTRODUCTION.....	6
1 Scope.....	9
2 Normative references	10
3 Terms and definitions	11
4 General	13
5 EMC test plan.....	14
5.1 General.....	14
5.2 Configuration of EUT during testing.....	14
5.2.1 General.....	14
5.2.2 Composition of EUT.....	14
5.2.3 Assembly of EUT.....	14
5.2.4 I/O ports.....	15
5.2.5 Auxiliary equipment.....	15
5.2.6 Cabling and earthing (grounding).....	15
5.3 Operation conditions of EUT during testing.....	15
5.3.1 Operation modes.....	15
5.3.2 Environmental conditions.....	15
5.3.3 EUT software during test.....	15
5.4 Specification of performance criteria.....	15
5.5 Test description.....	15
6 Performance criteria	16
6.1 Performance criteria A, B and C.....	16
6.2 Performance criterion FS.....	16
6.3 Application of the performance criterion FS.....	16
7 Immunity requirements	16
8 Test set-up and test philosophy for EUT with functions intended for safety applications.....	19
8.1 Testing of safety-related systems and equipment intended to be used in safety-related systems	19
8.2 Test philosophy for equipment intended for use in safety-related systems.....	20
8.3 Test philosophy for safety-related systems.....	20
8.4 Test configuration.....	20
8.5 Monitoring	21
9 Test results and test report.....	21
Annex A (informative) Evaluation of electromagnetic phenomena	25
Annex B (informative) Details of the specified electromagnetic environment	27
Annex C (informative) Example of immunity levels in the process industry.....	31
Bibliography.....	32
Figure 1 – Correlation between the standards IEC 61326-1, IEC 61326-2-X, IEC 61326-3-1 and IEC 61326-3-2	8

Figure 2 – Typical test set-up for equipment intended for use in a safety related system integrated into a representative safety-related system during test	22
Figure 3 – Typical test set-up for equipment intended for use in a safety-related system tested stand-alone	23
Figure 4 – Test set-up for a safety-related system	24
Figure B.1 – Recommended cable layouts for different categories	28
Table 1a – Immunity test requirements for equipment intended for use in industrial locations with specified electromagnetic environment – Enclosure port	17
Table 1b – Immunity test requirements for equipment intended for use in industrial locations with specified electromagnetic environment – Input and output a.c. power ports	17
Table 1c – Immunity test requirements for equipment intended for use in industrial locations with specified electromagnetic environment – Input and output d.c. power ports	18
Table 1d – Immunity test requirements for equipment intended for use in industrial locations with specified electromagnetic environment – I/O signal/control ports	18
Table 1e – Immunity test requirements for equipment intended for use in industrial locations with specified electromagnetic environment – I/O signal/control ports connected directly to power supply networks	19
Table 1f – Immunity test requirements for equipment intended for use in industrial locations with specified electromagnetic environment – Functional earth port	19
Table A.1 – General considerations for the application of electromagnetic phenomena for functional safety in industrial applications with specified electromagnetic environment (examples)	26
Table C.1 – Immunity test requirements for equipment intended for use in industrial locations with a specified electromagnetic environment according to NE 21	31

Document for review generated by EVS

INTERNATIONAL ELECTROTECHNICAL COMMISSION

ELECTRICAL EQUIPMENT FOR MEASUREMENT, CONTROL AND LABORATORY USE – EMC REQUIREMENTS –

Part 3-2: Immunity requirements for safety-related systems and for equipment intended to perform safety-related functions (functional safety) – Industrial applications with specified electromagnetic environment

FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC provides no marking procedure to indicate its approval and cannot be rendered responsible for any equipment declared to be in conformity with an IEC Publication.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

International Standard IEC 61326-3-2 has been prepared by subcommittee 65A, System aspects, of IEC technical committee 65: Industrial-process measurement and control.

The IEC 61326 series cancels and replaces IEC 61326:2002 and constitutes a technical revision.

IEC 61326-3-2 is to be read in conjunction with IEC 61326-1.

The text of this standard is based on the following documents:

FDIS	Report on voting
65A/501/FDIS	65A/506/RVD

Full information on the voting for the approval of this standard can be found in the report on voting indicated in the above table.

This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.

A list of all the parts of the IEC 61326 series, under the general title *Electrical equipment for measurement, control and laboratory use – EMC requirements*, can be found on the IEC website.

The committee has decided that the contents of this publication will remain unchanged until the maintenance result date indicated on the IEC web site under "<http://webstore.iec.ch>" in the data related to the specific publication. At this date, the publication will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

INTRODUCTION

Functional safety is that part of the overall safety relating to the equipment under control (EUC) and the EUC control system which depends on the correct functioning of the electrical safety-related systems. To achieve this all items of equipment of the safety-related system which are involved in the performance of the safety functions must behave in a specified manner under all relevant conditions.

The IEC basic safety publication for functional safety of electrical/electronic/programmable electronic safety-related systems is IEC 61508. It sets the overall requirements to achieve functional safety. Sufficient immunity to electromagnetic disturbances is one of those requirements.

The concept of IEC 61508 distinguishes between the consideration of the application and the design of safety-related electrical and electronic systems. The interface between both is the safety requirements specification (SRS). It specifies all relevant requirements of the intended application, as follows.

- a) Definition of the safety function, based on a risk assessment of the intended application (which function is intended to reduce risk).
- b) Appropriate safety integrated level (SIL) for each safety-function based on a risk assessment of the intended application.
- c) Definition of the environment in which the system is intended to work including the electromagnetic environment as required by IEC 61508-2.

Hence, with regard to immunity against electromagnetic phenomena, the essential starting point is that the electromagnetic environment and its phenomena are considered in the SRS, as required by IEC 61508. The safety-related system intended to implement the specified safety-function has to fulfil the SRS, and from it corresponding immunity requirements have to be derived for the items of equipment; this results in an equipment requirement specification. With respect to the electromagnetic environment, the SRS and the equipment requirement specification should be based on a competent assessment of the foreseeable electromagnetic threats in the real environment over the whole operational life of the equipment. Hence immunity requirements for the equipment depend on the characteristics of the electromagnetic environment in which the equipment is intended to be used.

The equipment manufacturer, therefore, has to prove that the equipment fulfils the equipment requirement specification and the system integrator must prove that the system fulfils the SRS. Evidence has to be produced by application of appropriate methods. They do not need to consider any other aspects of the application, for example risk of the application associated to any failure of the safety-related system. The objective is for all equipment in the system to comply with particular performance criteria taking into account functional safety aspects (for example the performance criterion FS) up to levels specified in the SRS independent of the required safety integrity level (SIL).

There are basically two approaches on how to deal with the electromagnetic environments and to conclude on immunity requirements.

- (A) To consider a general electromagnetic environment with no specific restrictions, for example an industrial environment, and to take into account all the electromagnetic phenomena that can occur as well as their maximum amplitudes when deriving appropriate immunity levels for the system and the equipment. This approach has been used to determine the levels specified within IEC 61326-3-1 leading to increased immunity levels for some electromagnetic phenomena compared to immunity levels which are derived without functional safety considerations.
- (B) To control the electromagnetic environment for example by the application of particular installation and mitigation practices, in such a way that electromagnetic phenomena and their amplitudes could occur only to a certain extent. These phenomena and restricted amplitudes are then taken into account by appropriate

immunity levels. These levels are not necessarily higher than those derived without functional safety considerations because it is ensured by corresponding means that no higher amplitudes as normally are to be expected. This approach is considered in this part of IEC 61326..

Applying approach (B) results in the fact that there is a specified electromagnetic environment due to the strict observation of particular installation and mitigation practices. In addition, however, appropriate knowledge is required concerning the electromagnetic phenomena and the amplitudes to be expected in this specified electromagnetic environment. This has been achieved by taking into account statistical data on faults in safety applications of the process industry. For this evaluation more than 20 000 units in safety applications are annually analysed on the occurrence of failures; from this data it has been shown that the failure rates meet the requirements connected to the safety integrity level (SIL). These units are in compliance with particular EMC requirements of the process industry.

Following approach (B), IEC 61326-3-2 gives specific electromagnetic immunity requirements that apply to safety-related systems and equipment intended to be used in safety-related systems. These requirements supplement some requirements of IEC 61326-1 (or of comparable EMC requirements of the process industry) and the selected electromagnetic phenomena and defined immunity test levels are expected to match with the environmental conditions of the specified industrial applications as defined in the scope of this standard.

The correlation between the standards IEC 61326-1, IEC 61326-2-X, IEC 61326-3-1 and IEC 61326-3-2 is described in the diagram of Figure 1.

The specified test levels in this standard are derived from the highest levels to be expected in the specified environment of industrial applications. These test levels are related to the electromagnetic environment (what can occur). They cannot be related in an analytical way to the SIL required for the safety-related system because there is no practically provable relationship between test level and probability of failure during use. The influences of electromagnetic phenomena are considered as systematic effects and by their nature often result in common cause events.

Design features of equipment must take into account the required SIL and must be designed to avoid dangerous systematic failures. Sufficient immunity against electromagnetic disturbances can only be ensured by design, mitigation and construction techniques which take into account electromagnetic aspects, which, however, are not within the scope of this standard.

It is therefore recommended that the approach to achieve the capability for the required SIL should be through the adoption of design features on the one hand and through appropriate test performance parameters in order to increase the level of confidence in the test results on the other hand.

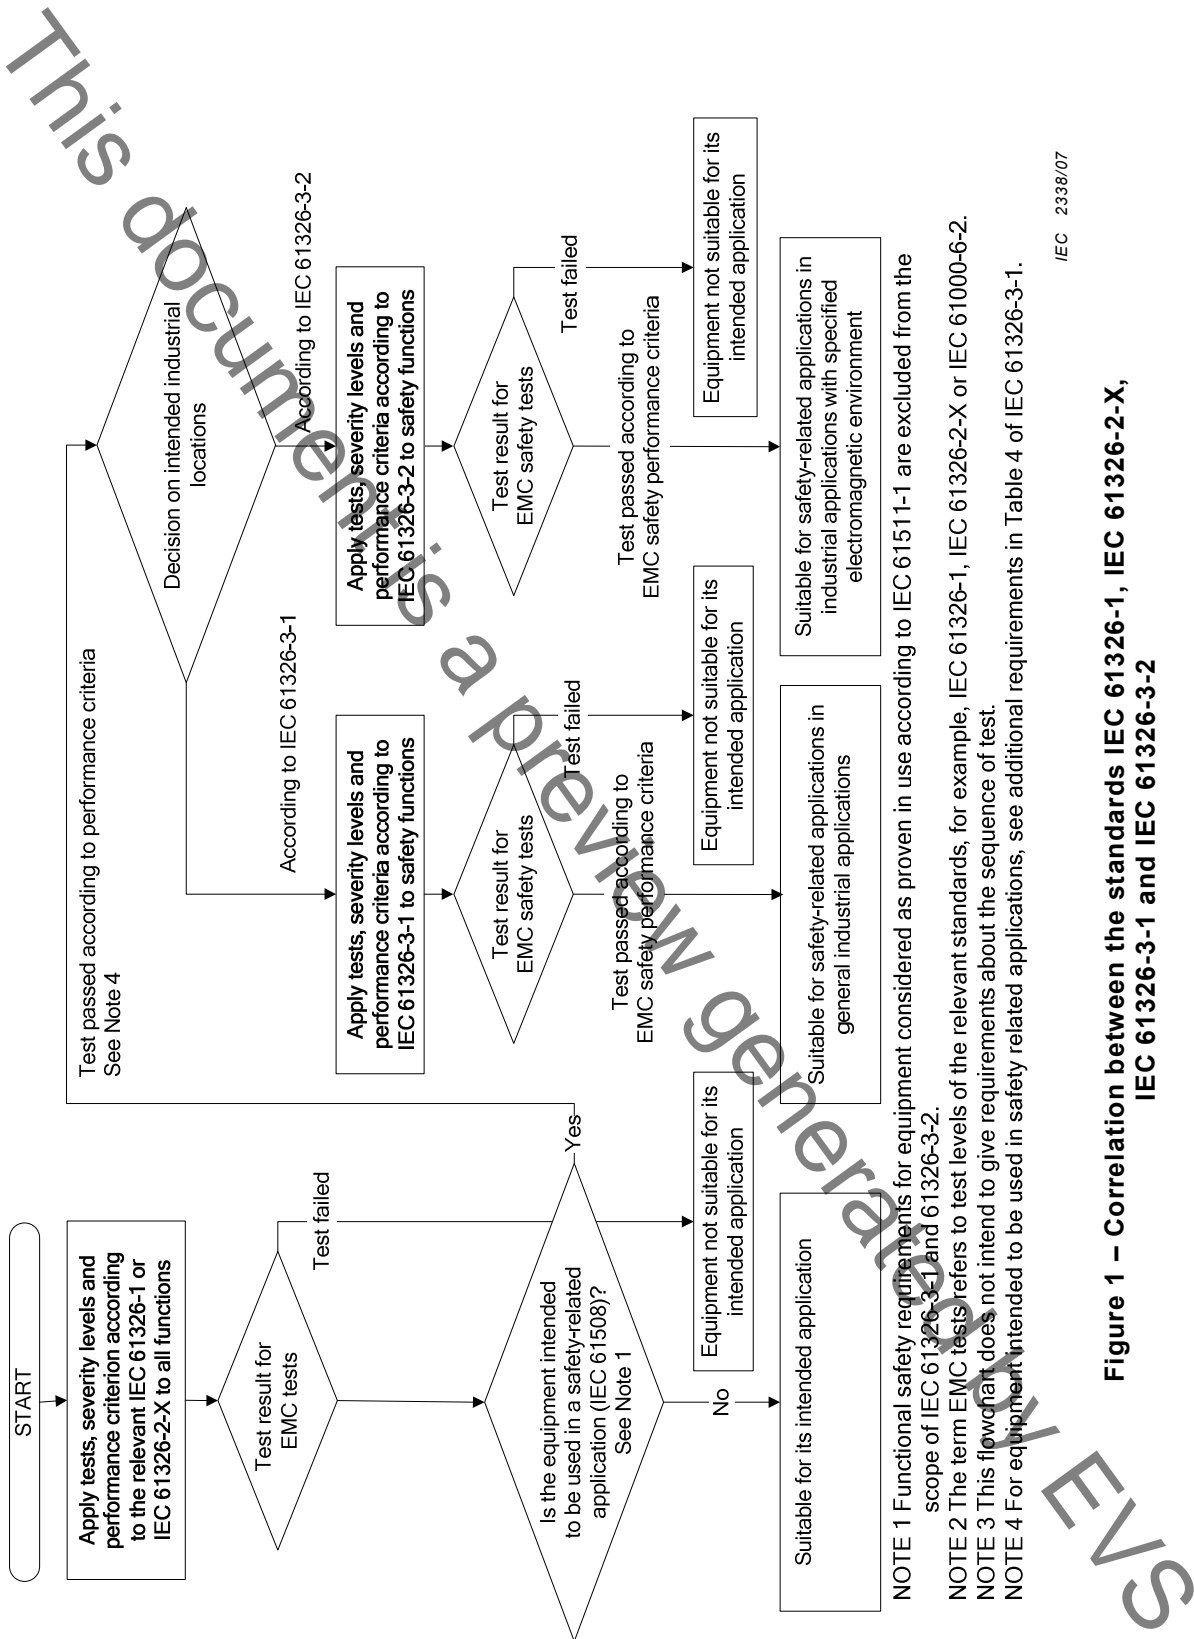


Figure 1 – Correlation between the standards IEC 61326-1, IEC 61326-2-X, IEC 61326-3-1 and IEC 61326-3-2

ELECTRICAL EQUIPMENT FOR MEASUREMENT, CONTROL AND LABORATORY USE – EMC REQUIREMENTS –

Part 3-2: Immunity requirements for safety-related systems and for equipment intended to perform safety-related functions (functional safety) – Industrial applications with specified electromagnetic environment

1 Scope

The scope of IEC 61326-1 applies to this part of IEC 61326 but is limited to systems and equipment for industrial applications within a specified electromagnetic environment and intended to perform safety functions as defined in IEC 61508 with SIL 1-3.

The electromagnetic environments encompassed by this product family standard are industrial, both indoor and outdoor, as they can be found in industrial applications with an electromagnetic environment having specified characteristics (for example, process industry). The difference between the electromagnetic environment covered by this standard compared to the general industrial environment (see IEC 61326-3-1) is due to the mitigation measures employed against electromagnetic phenomena leading to a specified electromagnetic environment.

The environment of industrial application with a specified electromagnetic environment typically includes the following characteristics:

- industrial area with limited access;
- limited use of mobile transmitter;
- dedicated cables for power supply and control, signal or communication lines;
- separation between power supply and control, signal or communication cables;
- factory building mostly consisting of metal construction;
- overvoltage/lightning protection by appropriate measures (for example, metal construction of the building or use of protection devices);
- pipe heating systems driven by a.c. main power may be present;
- no high-voltage substation close to sensitive areas;
- presence of CISPR 11 Group 2 ISM equipment using ISM frequencies only with low power;
- competent staff;
- periodical maintenance of equipment and systems;
- mounting and installation guidelines for equipment and systems.

A more detailed description of the above-mentioned typical characteristics is given in Annex B.

Equipment and systems considered as “proven-in-use” according to IEC 61508 or IEC 61511 are excluded from the scope of IEC 61326-3-2.

Fire alarm systems and security alarm systems intended for protection of buildings are excluded from the scope of IEC 61326-3-2.

2 Normative references

The following referenced documents are indispensable for the application of this standard. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

IEC 60050-161, *International Electrotechnical Vocabulary – Chapter 161: Electromagnetic compatibility*

IEC 61000-4-2:2001, *Electromagnetic compatibility (EMC) – Part 4-2: Testing and measurement techniques – Electrostatic discharge immunity test*

IEC 61000-4-3:2006, *Electromagnetic compatibility (EMC) – Part 4-3: Testing and measurement techniques – Radiated, radio-frequency, electromagnetic field immunity test*

IEC 61000-4-4:2004, *Electromagnetic compatibility (EMC) – Part 4-4: Testing and measurement techniques – Electrical fast/transient burst immunity test*

IEC 61000-4-5:2005, *Electromagnetic compatibility (EMC) – Part 4-5: Testing and measurement techniques – Surge immunity test*

IEC 61000-4-6:2004, *Electromagnetic compatibility (EMC) – Part 4-6: Testing and measurement techniques – Immunity to conducted disturbances, induced by radio-frequency fields*

IEC 61000-4-8:1993, *Electromagnetic compatibility (EMC) – Part 4-8: Testing and measurement techniques – Power frequency magnetic field immunity test¹*

Amendment 1 (2000)

IEC 61000-4-11:2004, *Electromagnetic compatibility (EMC) – Part 4-11: Testing and measurement techniques – Voltage dips, short interruptions and voltage variations immunity tests*

IEC 61000-4-29:2000, *Electromagnetic compatibility (EMC) – Part 4-29: Testing and measurement techniques – Voltage dips, short interruptions and voltage variations on d.c. input power port immunity tests*

IEC 61000-6-2:2005, *Electromagnetic compatibility (EMC) – Part 6-2: Generic standards – Immunity for industrial environments*

IEC 61326-1:2005, *Electrical equipment for measurement, control and laboratory use – EMC requirements – Part 1: General requirements*

IEC 61326-2-1:2005, *Electrical equipment for measurement, control and laboratory use – EMC requirements – Part 2-1: Particular requirements – Test configurations, operational conditions and performance criteria for sensitive test and measurement equipment for EMC unprotected applications*

IEC 61326-2-2:2005, *Electrical equipment for measurement, control and laboratory use – EMC requirements – Part 2-2: Particular requirements – Test configurations, operational conditions and performance criteria for portable test, measuring and monitoring equipment used in low-voltage distribution systems*

IEC 61326-2-3:2006, *Electrical equipment for measurement, control and laboratory use – EMC requirements – Part 2-3: Particular requirements – Test configurations, operational*

¹ There exists a consolidated edition 1.1 (2001) that includes edition 1.0 and its amendment.

conditions and performance criteria for transducers with integrated or remote signal conditioning

IEC 61326-2-4:2006, *Electrical equipment for measurement, control and laboratory use – EMC requirements – Part 2-4: Particular requirements – Test configurations, operational conditions and performance criteria for insulation monitoring devices according to IEC 61557-8 and for equipment for insulation fault location according to IEC 61557-9*

IEC 61326-2-5:2006, *Electrical equipment for measurement, control and laboratory use – EMC requirements – Part 2-5: Particular requirements – Test configurations, operational conditions and performance criteria for field devices with interfaces according to IEC 61784-1, CP 3/2*

IEC 61326-3-1:2008, *Electrical equipment for measurement, control and laboratory use – EMC requirements – Part 3-1: Immunity requirements for safety-related systems and for equipment intended to perform safety functions (functional safety) – General industrial applications*

IEC 61508-2:2000, *Functional safety of electrical/electronic/programmable electronic safety-related systems – Part 2: Requirements for electrical/electronic/programmable electronic safety-related systems*

IEC 61508-4:1998, *Functional safety of electrical/electronic/programmable electronic safety-related systems – Part 4: Definitions and abbreviations*

IEC 61511-1:2003, *Functional safety – Safety instrumented systems for the process industry sector – Part 1: Framework, definitions, system, hardware and software requirements*

ISO/IEC Guide 51:1999, *Safety aspects – Guidelines for their inclusion in standards*

3 Terms and definitions

For the purposes of this document, the terms and definitions of IEC 61326-1 and IEC 60050-161, as well as the following, apply.

NOTE Other definitions not included in IEC 60050-161 and in this standard, but nevertheless necessary for the application of the different tests, are given in the EMC basic publications of the IEC 61000 series.

3.1

dangerous failure

failure which has the potential to put the safety-related system in a hazardous or fail-to-function state

NOTE Whether or not the potential is realised may depend on the channel architecture of the system; in systems with multiple channels to improve safety, a dangerous hardware failure is less likely to lead to the overall dangerous or fail-to-function state.

[IEC 61508-4, 3.6.7]

3.2

equipment

the term equipment as used in this document is extremely general and is applied to a wide variety of possible sub-systems, apparatus, appliances and other assemblies of products.

3.3

equipment under control (EUC)

equipment, machinery, apparatus or plant used for manufacturing, process, transportation, medical or other activities