

**Steriilsed ühekordselt kasutatavad intravaskulaarsed
(soonesised) kateetrid. Osa 4:
Balloondilatatsioonikateetrid**

**Intravascular catheters - Sterile and single-use catheters
- Part 4: Balloon dilatation catheters (ISO 10555-4:2013)**

EESTI STANDARDI EESSÕNA

NATIONAL FOREWORD

See Eesti standard EVS-EN ISO 10555-4:2013 sisaldab Euroopa standardi EN ISO 10555-4:2013 ingliskeelset teksti.	This Estonian standard EVS-EN ISO 10555-4:2013 consists of the English text of the European standard EN ISO 10555-4:2013.
Standard on jõustunud sellekohase teate avaldamisega EVS Teatajas.	This standard has been endorsed with a notification published in the official bulletin of the Estonian Centre for Standardisation.
Euroopa standardimisorganisatsioonid on teinud Euroopa standardi rahvuslikele liikmetele kättesaadavaks 10.07.2013.	Date of Availability of the European standard is 10.07.2013.
Standard on kättesaadav Eesti Standardikeskusest.	The standard is available from the Estonian Centre for Standardisation.

Tagasisidet standardi sisu kohta on võimalik edastada, kasutades EVS-i veebilehel asuvat tagasiside vormi või saates e-kirja meiliaadressile standardiosakond@evs.ee.

ICS 11.040.25

Standardite reprodutseerimise ja levitamise õigus kuulub Eesti Standardikeskusele

Andmete paljundamine, taastekitamine, kopeerimine, salvestamine elektroonsesse süsteemi või edastamine ükskõik millises vormis või millisel teel ilma Eesti Standardikeskuse kirjaliku loata on keelatud.

Kui Teil on küsimusi standardite autorikaitse kohta, võtke palun ühendust Eesti Standardikeskusega:
Aru 10, 10317 Tallinn, Eesti; www.evs.ee; telefon 605 5050; e-post info@evs.ee

The right to reproduce and distribute standards belongs to the Estonian Centre for Standardisation

No part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying, without a written permission from the Estonian Centre for Standardisation.

If you have any questions about copyright, please contact Estonian Centre for Standardisation:
Aru 10, 10317 Tallinn, Estonia; www.evs.ee; phone 605 5050; e-mail info@evs.ee

English Version

Intravascular catheters - Sterile and single-use catheters - Part
4: Balloon dilatation catheters (ISO 10555-4:2013)

Cathéters intravasculaires - Cathéters stériles et non
réutilisables - Partie 4: Cathéters de dilatation à ballonnets
(ISO 10555-4:2013)

Intravaskuläre Katheter - Sterile Katheter zur einmaligen
Verwendung - Teil 4: Ballondilatationskatheter (ISO 10555-
4:2013)

This European Standard was approved by CEN on 29 May 2013.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN-CENELEC Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN-CENELEC Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: Avenue Marnix 17, B-1000 Brussels

Foreword

This document (EN ISO 10555-4:2013) has been prepared by Technical Committee ISO/TC 84 “Devices for administration of medicinal products and intravascular catheters” in collaboration with Technical Committee CEN/TC 205 “Non-active medical devices” the secretariat of which is held by DIN.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by January 2014, and conflicting national standards shall be withdrawn at the latest by January 2014.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

This document supersedes EN ISO 10555-4:1997.

This document has been prepared under a mandate given to CEN by the European Commission and the European Free Trade Association, and supports essential requirements of EU Directive(s).

For relationship with EU Directive(s), see informative Annex ZA, which is an integral part of this document.

According to the CEN-CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and the United Kingdom.

Endorsement notice

The text of ISO 10555-4:2013 has been approved by CEN as EN ISO 10555-4:2013 without any modification.

Annex ZA (informative)

Relationship between this European Standard and the Essential Requirements of EU Directive 93/42/EEC amended by Directive 2007/47/EEC

This European Standard has been prepared under a mandate given to CEN by the European Commission and the European Free Trade Association to provide a means of conforming to Essential Requirements of Directive 93/42/EEC amended by Directive 2007/47/EEC.

Once this standard is cited in the Official Journal of the European Union under that Directive and has been implemented as a national standard in at least one Member State, compliance with the normative clauses of this standard given in Table ZA.1 confers, within the limits of the scope of this standard, a presumption of conformity with the relevant Essential Requirements of that Directive.

NOTE When an Essential Requirement does not appear in Table ZA.1, it means that it is not addressed by this European Standard.

Table ZA.1— Correspondence between this European Standard and Directive 93/42/EEC amended by Directive 2007/47/EEC

Essential Requirements (ERs) of Directive 93/42/EEC	Clause(s)/sub-clause(s) of this EN ISO 10555-4
7.3	4.1 4.4
7.5	4.1
8.1	4.1
8.3	4.1
8.4	4.1
9.1	4.1
9.2	4.1 4.2 4.3 4.4
12.7.1	4.1 4.4
12.7.4	4.1
12.8.1	4.1
13.1	4.1 4.5 a)
13.2	4.1
13.3 a)	4.1
13.3 b)	4.1

13.3 c)	4.1
13.3 d)	4.1
13.3 e)	4.1
13.3 f)	4.1
13.3 i)	4.1
13.3 j)	4.1 4.5 b), c), d) and e)
13.3 k)	4.1
13.3 m)	4.1
13.4	4.1
13.6 a)	4.1
13.6 b)	4.1 4.5 a), b) and c)
13.6 c)	4.1
13.6 e)	4.1
13.6 f)	4.1
13.6 g)	4.1
13.6 k)	4.1
13.6 l)	4.1
13.6 n)	4.1
13.6 q)	4.1

WARNING — Other requirements and other EU Directives may be applicable to the product(s) falling within the scope of this standard.

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Requirements	1
4.1 General.....	1
4.2 Radio-detectability.....	1
4.3 Designation of nominal size.....	1
4.4 Physical requirements.....	2
4.5 Information to be supplied by the manufacturer.....	2
Annex A (normative) Test for balloon rated burst pressure (RBP)	3
Annex B (normative) Balloon fatigue test for freedom from leakage and damage on inflation	5
Annex C (normative) Test for balloon deflation time	7
Annex D (normative) Test for balloon diameter to inflation pressure	9
Annex E (informative) Guidance on the selection of balloon materials	11
Bibliography	12

Intravascular catheters — Sterile and single-use catheters —

Part 4: Balloon dilatation catheters

1 Scope

This part of ISO 10555 specifies requirements for balloon dilatation catheters supplied in the sterile condition, and intended for single use.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 594-1, *Conical fittings with a 6 % (Luer) taper for syringes, needles and certain other medical equipment — Part 1: General requirements*¹⁾

ISO 594-2, *Conical fittings with a 6 % (Luer) taper for syringes, needles and certain other medical equipment — Part 2: Lock fittings*¹⁾

ISO 10555-1, *Intravascular catheters — Sterile and single-use catheters — Part 1: General requirements*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 10555-1 and the following apply.

3.1

balloon dilatation catheter

intravascular catheter fitted with a balloon near the distal end, which is introduced into an artery or vein to dilate a part or parts of the vascular system

4 Requirements

4.1 General

Unless otherwise specified in this part of ISO 10555, balloon dilatation catheters shall comply with ISO 10555-1.

4.2 Radio-detectability

The position of the balloon shall be radio detectable when the catheter has been inserted into the body.

4.3 Designation of nominal size

The nominal size of the catheter shall be designated by the following:

- a) diameter(s) expressed in millimetres of the inflated balloon(s) or, for multidiameter balloon(s), the diameter of each portion at recommended pressure;

1) Upon its publication, ISO 80369-7 will replace ISO 594-1 and ISO 594-2.

- b) effective length of the balloon at recommended pressure;
- c) diameter of the largest guidewire that can be used with the catheter, if applicable.

NOTE Where a balloon dilation catheter (see Figure B.1) is used as a stent delivery system, refer to the appropriate standard for stents for designation of nominal size.

4.4 Physical requirements

4.4.1 Balloon rated burst pressure (RBP)

Determine the burst pressure with an appropriate safety margin when tested in accordance with [Annex A](#). Longitudinal failure is the desirable balloon failure mode.

4.4.2 Balloon fatigue; freedom from leakage and damage on inflation

Evaluate the ability of the balloon to withstand repeated inflation cycles to the RBP. When tested as described in [Annex B](#), there shall be no leakage or evidence of damage, such as herniation or bursting of the catheter.

4.4.3 Balloon deflation time

Determine the time required to deflate the balloon from the RBP as described in [Annex C](#).

4.4.4 Balloon diameter to inflation pressure

Determine the relationship between the balloon diameter and the balloon inflation pressure as described in [Annex D](#).

4.5 Information to be supplied by the manufacturer

Information supplied by the manufacturer shall comply with ISO 10555-1 and shall also include the following:

- a) nominal size of the catheter, as designated in [4.3](#);
- b) position(s) of radio-detectable marker(s);
- c) RBP of the balloon, expressed in kilopascals;
- d) balloon inflation pressure, expressed in kilopascals, required to achieve the nominal balloon diameter(s);
- e) guidewire, guide catheter or sheath or introducer compatibility and size recommendations appropriate to the intended clinical use.

NOTE Units of measurement systems other than those specified in this part of ISO 10555 can additionally be used.

Annex A

(normative)

Test for balloon rated burst pressure (RBP)

A.1 Principle

The purpose of this test is to determine the RBP of the balloon.

A.2 Apparatus

A.2.1 Recommended guidewire or equivalent.

A.2.2 Water bath, controlled at $(37 \pm 2) ^\circ\text{C}$.

A.2.3 Leak detection mechanism, e.g. dye in test fluid, pressure drop monitor, flow rate monitor.

A.2.4 Fluid for inflation, e.g. room temperature water or other justified clinically relevant media.

A.2.5 Timing mechanism, with specified accuracy.

A.2.6 Pressure generating device, fitted with a means of measuring pressure with an accuracy of $\pm 5\%$ of the reported value and maintaining the inflation pressure and fitted with a male 6 % (Luer) taper, complying with ISO 594-1 or ISO 594-2 as applicable, for connection to the catheter.

A.3 Test procedure

A.3.1 Fill the pressure generating device (A.2.6) with fluid for inflation.

A.3.2 If the instructions for use specify that a guidewire should be used during balloon inflation, insert the appropriate guidewire (A.2.1) in the device.

A.3.3 Connect the pressure generating device to the catheter under test and immerse at least the whole of the balloon portion(s) in the water bath (A.2.2) at $(37 \pm 2) ^\circ\text{C}$.

A.3.4 Allow the catheter to equilibrate for a minimum of 2 min.

A.3.5 Inflate the balloon using a pre-determined pressure profile versus time until the catheter bursts or fails. Record the burst pressure, failure mode and location of the failure.

A.4 Test report

The test report shall include the following information:

- a) identity of the catheter;
- b) mean burst pressure, RBP and maximum, minimum and standard deviation of the burst data, expressed in kilopascals;

- c) all observed failure modes.

NOTE Units of measurement systems other than those specified in this part of ISO 10555 can additionally be used.

This document is a preview generated by EVS

Annex B

(normative)

Balloon fatigue test for freedom from leakage and damage on inflation

B.1 Principle

The catheter is inflated and deflated a number of times to simulate use *in vivo*. The catheter in an inflated condition is examined for leakage, rupture or herniation.

B.2 Apparatus

B.2.1 Recommended guidewire or equivalent.

B.2.2 Water bath, controlled at $(37 \pm 2) ^\circ\text{C}$.

B.2.3 Leak detection mechanism, e.g. dye in test fluid, pressure drop monitor, flow rate monitor.

B.2.4 Timing mechanism, with specified accuracy.

B.2.5 Inflation syringe or equivalent device, fitted with a means of measuring pressure with an accuracy of $\pm 5\%$ of the reported value and maintaining the inflation pressure and fitted with a male 6 % (Luer) taper, complying with ISO 594-1 or ISO 594-2 as applicable, for connection to the catheter.

B.2.6 Compliant tube (if applicable, with a clinically relevant compliance and rationale for use, e.g. when measuring within a stent) of a diameter that represents the recommended vessel diameter for the catheter under test in order to keep the device from moving excessively during inflation cycles.

B.3 Test procedure

B.3.1 Fill the inflation device (B.2.5) with water or other clinically relevant media (selection of media to be justified).

B.3.2 If the instructions for use specify that a guidewire should be used during balloon inflation, insert the appropriate guidewire (A.2.1) in the device.

B.3.3 Connect the inflation device to the catheter under test and immerse at least the whole of the balloon portion(s) in the water bath (B.2.2) at $(37 \pm 2) ^\circ\text{C}$. If a compliant tube is being used, insert device into the compliant tube.

B.3.4 Allow the catheter to equilibrate for a minimum of 2 min. Inflate it to RBP holding the inflation pressure for a minimum of 30 s before deflating. Then deflate the balloon(s). Repeat this procedure eight times. Observe for leaks.

B.3.5 After a total of 9 times of inflation/deflation according to B.3.4, inflate the balloon(s) further one time to the RBP and remove the catheter from the water bath, maintaining the balloon(s) in the inflated state.


B.3.6 Inspect the whole catheter for leakage, rupture, herniation, direction of any balloon rupture, and, if rupture occurred, whether fragments were produced.

B.4 Test report

The test report shall include the following information:

- identity of the catheter;
- inflation pressure used, expressed in kilopascals;
- whether leakage occurred from the catheter;
- whether the catheter shaft or balloon(s) ruptured or herniated, the direction of any balloon rupture, and, if rupture occurred, whether fragments were produced.

NOTE Units of measurement systems other than those specified in this part of ISO 10555 can additionally be used.

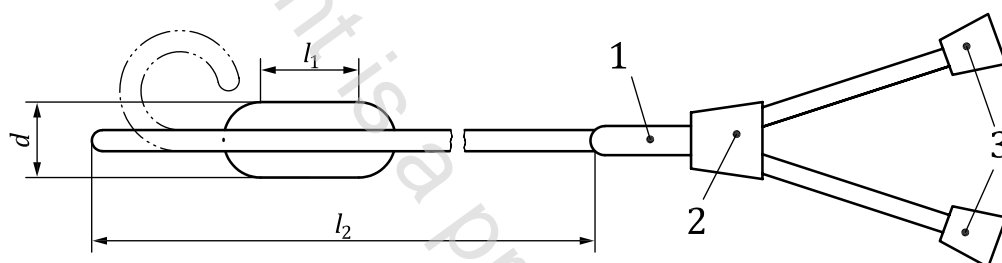

Key

- d inflated balloon diameter
- l_1 effective length of the balloon
- l_2 effective length of the catheter
- 1** catheter strain reinforcement
- 2** junction
- 3** catheter hub(s)

NOTE This drawing shows the designation of dimensions, but the representation of the components is schematic only.

Figure B.1 — Designation of dimensions of balloon dilatation catheter