

Health informatics - Personal health device communication - Part 20601: Application profile - Optimized exchange protocol (ISO/IEEE 11073-20601:2010)

EESTI STANDARDI EESSÕNA

NATIONAL FOREWORD

Käesolev Eesti standard EVS-EN ISO 11073-20601:2011 sisaldb Euroopa standardi EN ISO 11073-20601:2011 ingliskeelset teksti.	This Estonian standard EVS-EN ISO 11073-20601:2011 consists of the English text of the European standard EN ISO 11073-20601:2011.
Standard on kinnitatud Eesti Standardikeskuse 31.03.2011 käskkirjaga ja jõustub sellekohase teate avaldamisel EVS Teatajas.	This standard is ratified with the order of Estonian Centre for Standardisation dated 31.03.2011 and is endorsed with the notification published in the official bulletin of the Estonian national standardisation organisation.
Euroopa standardimisorganisatsioonide poolt rahvuslikele liikmetele Euroopa standardi teksti kätesaadavaks tegemise kuupäev on 16.03.2011.	Date of Availability of the European standard text 16.03.2011.
Standard on kätesaadav Eesti standardiorganisatsionist.	The standard is available from Estonian standardisation organisation.

ICS 35.240.80

Standardite reproduutseerimis- ja levitamisõigus kuulub Eesti Standardikeskusele

Andmete paljundamine, taastekitamine, kopeerimine, salvestamine elektroonilisse süsteemi või edastamine ükskõik millises vormis või millisel teel on keelatud ilma Eesti Standardikeskuse poolt antud kirjaliku loata.

Kui Teil on küsimusi standardite autorikaitse kohta, palun võtke ühendust Eesti Standardikeskusega:
Aru 10 Tallinn 10317 Estonia; www.evs.ee; Telefon: 605 5050; E-post: info@evs.ee

Right to reproduce and distribute belongs to the Estonian Centre for Standardisation

No part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying, without permission in writing from Estonian Centre for Standardisation.

If you have any questions about standards copyright, please contact Estonian Centre for Standardisation:
Aru str 10 Tallinn 10317 Estonia; www.evs.ee; Phone: 605 5050; E-mail: info@evs.ee

EUROPEAN STANDARD

EN ISO 11073-20601

NORME EUROPÉENNE

EUROPÄISCHE NORM

March 2011

ICS 35.240.80

English Version

Health informatics - Personal health device communication -
Part 20601: Application profile - Optimized exchange protocol
(ISO/IEEE 11073-20601:2010)

Informatique de santé - Communication entre dispositifs de santé personnels - Partie 20601: Profil d'application - Protocole d'échange optimisé (ISO/IEEE 11073-20601:2010)

Medizinische Informatik - Kommunikation von Geräten für die persönliche Gesundheit - Teil 20601: Anwendungsprofil - Optimiertes Datenübertragungsprotokoll (ISO/IEEE 11073-20601:2010)

This European Standard was approved by CEN on 23 April 2010.

CEN members are bound to comply with the CEN-CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN-CENELEC Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN-CENELEC Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: Avenue Marnix 17, B-1000 Brussels

Foreword

The text of ISO/IEEE 11073-20601:2010 has been prepared by Technical Committee ISO/TC 215 "Health informatics" of the International Organization for Standardization (ISO) and has been taken over as EN ISO 11073-20601:2011 by Technical Committee CEN/TC 251 "Health informatics" the secretariat of which is held by NEN.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by September 2011, and conflicting national standards shall be withdrawn at the latest by September 2011.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland and the United Kingdom.

Endorsement notice

The text of ISO/IEEE 11073-20601:2010 has been approved by CEN as a EN ISO 11073-20601:2011 without any modification.

Contents

	Page
Foreword.....	vi
Introduction.....	viii
1. Overview.....	1
1.1 Scope.....	1
1.2 Purpose.....	1
1.3 Context.....	2
2. Normative references.....	5
3. Definitions, acronyms, and abbreviations.....	5
3.1 Definitions.....	5
3.2 Acronyms and abbreviations.....	5
4. Guiding principles.....	6
5. Introduction to IEEE 11073 personal health devices.....	7
5.1 General.....	7
5.2 Domain information model (DIM).....	8
5.3 Service model.....	8
5.4 Communication model.....	8
6. Personal health device DIM.....	8
6.1 General.....	8
6.2 Nomenclature usage.....	9
6.3 Personal health object class definitions.....	10
6.3.1 General	10
6.3.2 MDS class	12
6.3.3 Metric class.....	18
6.3.4 Numeric class.....	23
6.3.5 RT-SA class.....	26
6.3.6 Enumeration class.....	27
6.3.7 PM-store class	30
6.3.8 PM-segment class	34
6.3.9 Scanner classes	37
6.4 Information model extensibility rules	45
7. Personal health device service model	45
7.1 General.....	45
7.2 Association service	46
7.3 Object access services	46
7.4 Specific application of object access EVENT REPORT services for personal health devices	47
7.4.1 General	47
7.4.2 Confirmed and unconfirmed event reports	47

7.4.3 Configuration event report	47
7.4.4 Agent- and manager-initiated measurement data transmission	49
7.4.5 Variable, fixed, and grouped format event reports	50
7.4.6 Single-person and multiple-person event reports	50
7.4.7 Temporarily stored measurements.....	51
 8. Communication model.....	52
8.1 General.....	52
8.2 System context	52
8.3 Communications characteristics.....	53
8.3.1 General	53
8.3.2 Common communications characteristics	55
8.3.3 Reliable communications characteristics	55
8.3.4 Best-effort communications characteristics.....	56
8.4 State machines.....	56
8.4.1 Agent state machine	56
8.4.2 Manager state machine	59
8.4.3 Timeout variables	60
8.5 Connected procedure.....	61
8.5.1 General	61
8.5.2 Entry conditions	61
8.5.3 Normal procedures	61
8.5.4 Exit conditions.....	61
8.5.5 Error conditions.....	62
8.6 Unassociated procedure	62
8.6.1 General	62
8.6.2 Entry conditions	62
8.6.3 Normal procedures	62
8.6.4 Exit conditions.....	62
8.6.5 Error conditions.....	62
8.7 Associating procedure.....	63
8.7.1 General	63
8.7.2 Entry conditions	63
8.7.3 Normal procedures	63
8.7.4 Exit conditions.....	67
8.7.5 Error conditions.....	67
8.7.6 Test association	67
8.8 Configuring procedure	69
8.8.1 General	69
8.8.2 Entry conditions	69
8.8.3 Normal procedures	69
8.8.4 Exit conditions.....	71
8.8.5 Error conditions.....	71
8.9 Operating procedure.....	72
8.9.1 General	72
8.9.2 Entry conditions	72
8.9.3 Normal procedures	72
8.9.4 Exit conditions.....	83
8.9.5 Error conditions.....	83
8.10 Disassociating procedure	85
8.10.1 General	85
8.10.2 Entry conditions	85
8.10.3 Normal procedures	85
8.10.4 Exit conditions.....	85
8.10.5 Error conditions.....	86
8.11 Message encoding	86
8.12 Time coordination	86

8.12.1 General	86
8.12.2 Absolute time	86
8.12.3 Relative time.....	88
8.12.4 High-resolution relative time.....	89
9. Conformance model.....	89
9.1 Applicability	89
9.2 Conformance specification.....	90
9.3 Implementation conformance statements (ICSSs)	90
9.4 General conformance	90
9.4.1 General ICS	91
9.4.2 Minimum requirements ICS	92
9.4.3 Service support ICS.....	93
9.5 Device additions/extensions ICS.....	94
9.5.1 General additions/extensions ICS.....	94
9.5.2 Personal health device DIM object and class (POC) ICS.....	95
9.5.3 POC attribute ICS.....	95
9.5.4 POC behavior ICS.....	96
9.5.5 POC notification ICS.....	96
9.5.6 POC nomenclature ICS.....	97
Annex A (normative) ASN.1 definitions.....	98
Annex B (informative) Scale and range specification example	130
Annex C (informative) The PM-store concept.....	132
Annex D (informative) Transport profile types	137
Annex E (normative) State tables	140
Annex F (normative) Medical device encoding rules (MDER)	151
Annex G (informative) Encoded data type definitions	163
Annex H (informative) Examples	182
Annex I (normative) Nomenclature codes	190
Annex J (informative) Derivation and modification history	194
Annex K (informative) Bibliography.....	197

Introduction

ISO and IEEE 11073 standards enable communication between medical devices and external computer systems. This standard and corresponding IEEE 11073-104zz standards address a need for a simplified and optimized communication approach for personal health devices, which may or may not be regulated devices. These standards align with, and draw upon, the existing clinically focused standards to provide easy management of data from either a clinical or personal health device.

This document addresses a need for an openly defined, independent standard for converting the collected information into an interoperable transmission format so the information can be exchanged between agents and managers.

Other closely related standards include the following:

- ISO/IEEE P11073-00103 [B6]^a provides an overview of the personal health space and defines the underlying use cases and usage models.
- ISO/IEEE 11073-10101 [B12] documents the nomenclature terms that can be used.
- ISO/IEEE 11073-10201:2004 [B13] documents the extensive domain information model (DIM) leveraged by this standard.
- ISO/IEEE 11073-104zz standards define specific device specializations. For example, ISO/IEEE P11073-10404 [B9] defines how interoperable pulse oximeters work.
- ISO/IEEE 11073-20101:2004 [B14] defines the medical device encoding rules (MDER) used in this standard.

^a The numbers in brackets correspond to the numbers of the bibliography in Annex K.

Health informatics — Point-of-care medical device communication —

Part 20601: Application profile — Optimized exchange protocol

IMPORTANT NOTICE: This standard is not intended to assure safety, security, health, or environmental protection in all circumstances. Implementers of the standard are responsible for determining appropriate safety, security, environmental, and health practices or regulatory requirements.

This IEEE document is made available for use subject to important notices and legal disclaimers. These notices and disclaimers appear in all publications containing this document and may be found under the heading "Important Notice" or "Important Notices and Disclaimers Concerning IEEE Documents." They can also be obtained on request from IEEE or viewed at <http://standards.ieee.org/IPR/disclaimers.html>.

1. Overview

1.1 Scope

Within the context of the ISO/IEEE 11073 family of standards for device communication, this standard defines a common framework for making an abstract model of personal health data available in transport-independent transfer syntax required to establish logical connections between systems and to provide presentation capabilities and services needed to perform communication tasks. The protocol is optimized to personal health usage requirements and leverages commonly used methods and tools wherever possible.

1.2 Purpose

This document addresses a need for an openly defined, independent standard for converting the information profile into an interoperable transmission format so the information can be exchanged to and from personal telehealth devices and compute engines (e.g., cell phones, personal computers, personal health appliances, and set top boxes).

1.3 Context

Figure 1 shows categories and typical devices supporting the personal health space. Agents (e.g., blood pressure monitors, weighing scales, and pedometers) collect information about a person (or persons) and transfer the information to a manager (e.g., cell phone, health appliance, or personal computer) for collection, display, and possible later transmission. The manager may also forward the data to remote support services for further analysis. The information is available from a range of domains including disease management, health and fitness, or aging independently applications.

The communication path between agent and manager is assumed to be a logical point-to-point connection. Generally, an agent communicates with a single manager at any point in time. A manager may communicate with multiple agents simultaneously using separate point-to-point connections.

The overlay shows the focus area of the IEEE 11073™ Personal Health Devices Working Group. The primary concentration is the interface and data exchange between the agents and manager. However, this interface cannot be created in isolation by ignoring the remainder of the solution space. Remaining cognizant of the entire system helps to ensure that data can reasonably move from the agents all the way to the remote support services when necessary. This path may include converting the data format, exchange protocols, and transport protocols across different interfaces. Much of the standardization effort is outside of the scope of the Personal Health Devices Working Group; however, aligning all standardization efforts allows data to flow seamlessly through the overall set of systems.

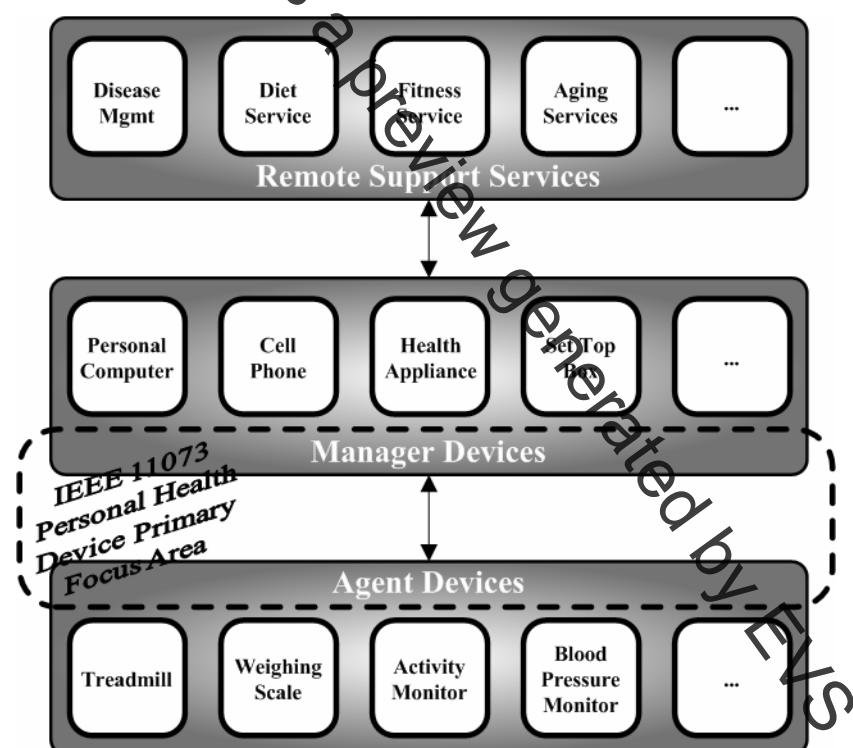


Figure 1 —Overall context of work

Figure 2 shows a hierarchical view of the architecture of an agent or manager superimposed with a view of the related standards. The application layers are, for the most part, not specific to any particular transport. Where necessary, this standard identifies assumptions that require direct support by a transport or a “shim” layer above the transport. This approach allows support for various transports. The definition of the transports is outside of the scope of this standard and the working group.

Above the transport layer is the Optimized Exchange Protocol (described in this standard). This protocol consists of two aspects: the application layer services and the definition of the data exchange protocol between agents and managers. The application layer services provide the protocol for connection management and reliable transfer of actions and data between agent and manager. The data exchange protocol defines the commands, agent configuration information, data format, and overall protocol. The Optimized Exchange Protocol provides the basis to support any type of agent. For a specific device type, the reader is directed to the device specialization for that agent to understand the capabilities of the device and its implementation according to this standard. The device specialization indicates which aspects of this standard to comprehend and where further information to implement the device is found.

Above the exchange protocol are device specializations that describe specific details relative to the particular agent (e.g., blood pressure monitor, weighing scale, or pedometer). The specializations describe the details of how these agents work and act as a detailed description for creating a specific type of agent. Additionally, they provide reference to a related standard for further details. The standard numbers reserved for device specializations range from IEEE Std 11073-10401 through IEEE Std 11073-10499, inclusive. When the collection of standards is being referenced, the term *IEEE 11073-104zz* is used where zz could be any number in the range from 01 to 99, inclusive.

The ISO/IEEE P11073-00103[¹] technical report describes the overall personal health space with further definition of the underlying use cases and usage models.

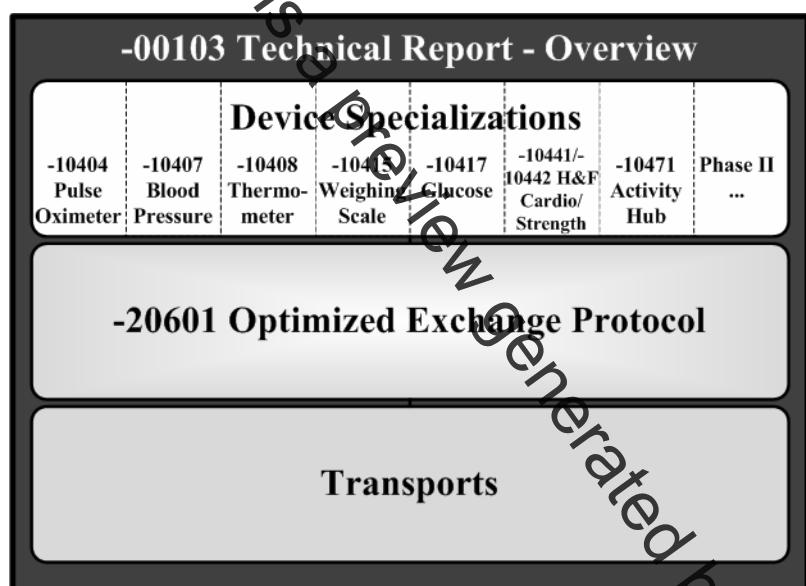


Figure 2 —Document map

The personal health device specializations are not being created independently of all other standards. There are a number of existing standards generated for clinical environments upon which these standards draw. Figure 3 shows the relationship to the remainder of the IEEE 11073 documents. There are two types of relationships:

¹ The numbers in brackets correspond to the numbers of the bibliography in Annex K.

- Drawing ideas and/or content from the other documents (dashed lines)
- Leveraging information from the other document and introducing new content into that document to support this standard (solid lines)

This standard imports information from ISO/IEEE 11073-10201:2004 [B13] and ISO/IEEE 11073-20101:2004 [B14] as normative annexes. If there is a discrepancy between these standards, this standard takes priority. Because of the reuse of constructs from these standards, some of the names appear to be more clinically focused [e.g., medical device system (MDS) instead of personal health device system]; however, to maintain consistency, the traditional names have been preserved.

This standard replicates relevant portions of ISO/IEEE 11073-10101 [B12] and incorporates new nomenclature codes.

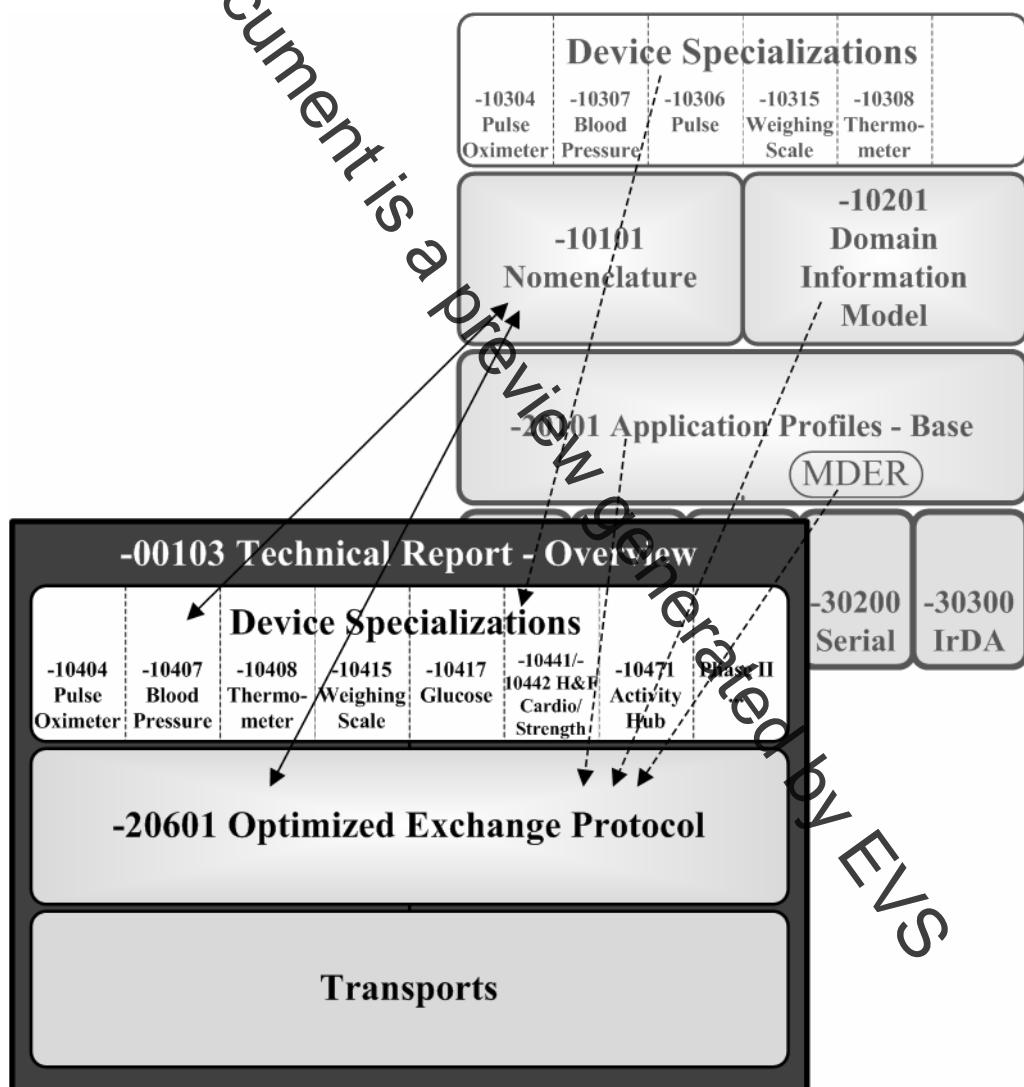


Figure 3 —Relationship to other IEEE 11073 documents

2. Normative references

The following referenced documents are indispensable for the application of this standard (i.e., they must be understood and used; therefore, each referenced document is cited in the text and its relationship to this standard is explained). For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments or corrigenda) applies.

IEEE Std 802®-2001, IEEE Standard for Local and Metropolitan Area Networks: Overview and Architecture.²

ITU-T Rec. X.667 (Sept. 2004), Information technology – Open Systems Interconnection – Procedures for the operation of OSI Registration Authorities: Generation and registration of universally unique identifiers (UUIDs) and their use as ASN.1 object identifier components.³

3. Definitions, acronyms, and abbreviations

3.1 Definitions

For the purposes of this standard, the following terms and definitions apply. *The Authoritative Dictionary of IEEE Standards* [B6] should be referenced for terms not defined in this clause.

3.1.1 agent: A node that collects and transmits personal health data to an associated manager.

3.1.2 compute engine: *See: manager.*

3.1.3 confirmed: An application-level, completion notification service mechanism. For EVENT REPORT services (i.e., the data plane), confirmation allows the agent to know when the manager has “accepted responsibility” for a piece of data so that the agent can delete that data. For the ACTION, GET, and SET services (i.e., the control plane), confirmation allows the manager to know when the agent has “completed” the requested transaction.

3.1.4 device: A physical device implementing either an agent or manager role.

3.1.5 handle: An unsigned 16-bit number that is locally unique and identifies one of the object instances within an agent.

3.1.6 manager: A node receiving data from one or more agent systems. Examples of managers include a cellular phone, health appliance, set top box, or computer system.

3.1.7 personal health device: A device used in personal health applications.

3.1.8 personal telehealth device: *See: personal health device.*

3.2 Acronyms and abbreviations

ASCII	American Standard Code for Information Interchange ⁴
ASN.1	Abstract Syntax Notation One
APDU	application protocol data unit

² IEEE publications are available from the Institute of Electrical and Electronics Engineers, 445 Hoes Lane, Piscataway, NJ 08854, USA (<http://standards.ieee.org/>).

³ ITU-T publications are available from the International Telecommunications Union, Place des Nations, CH-1211, Geneva 20, Switzerland/Suisse (<http://www.itu.int/>).

⁴ Note that throughout this standard the term ASCII is used to mean the character set as defined in ISO/IEC 646 (1991) [B7].