

---

---

**Indoor air —**

**Part 6:**

**Determination of organic compounds  
(VVOC, VOC, SVOC) in indoor and test  
chamber air by active sampling on  
sorbent tubes, thermal desorption and  
gas chromatography using MS or MS  
FID**

*Air intérieur —*

*Partie 6: Dosage des composés organiques (COTV, COV, COSV) dans  
l'air intérieur et l'air de chambre d'essai par prélèvement actif sur  
tubes à sorbant, désorption thermique et chromatographie en phase  
gazeuse avec détection MS ou MS-FID*



This document is a preview generated by EKO



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2021

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
CP 401 • Ch. de Blandonnet 8  
CH-1214 Vernier, Geneva  
Phone: +41 22 749 01 11  
Email: [copyright@iso.org](mailto:copyright@iso.org)  
Website: [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

Page

<b>Foreword</b>	<b>iv</b>
<b>Introduction</b>	<b>v</b>
<b>1 Scope</b>	<b>1</b>
<b>2 Normative references</b>	<b>1</b>
<b>3 Terms and definitions</b>	<b>1</b>
<b>4 Abbreviated terms</b>	<b>3</b>
<b>5 Principle</b>	<b>3</b>
<b>6 Reagents and materials</b>	<b>3</b>
<b>7 Apparatus</b>	<b>5</b>
<b>8 Conditioning and storage of sorbent tubes</b>	<b>9</b>
8.1 Conditioning	9
8.2 Storage of conditioned sorbent tubes before sampling	10
<b>9 Sampling</b>	<b>10</b>
9.1 Air sampling	10
9.2 Sampling volumes	10
9.3 Storage of loaded samples	11
9.4 Field blanks	11
<b>10 Analysis</b>	<b>11</b>
10.1 Determination of VOC, VVOC and SVOC	11
10.1.1 Analytical System	11
10.1.2 Identification of target compounds	13
10.1.3 Quantification of target compounds and compounds according to task list	14
10.1.4 Determining the lower limit of quantification	15
10.2 Identified non-target compounds and unidentified compounds	16
<b>11 Concentration of analytes in the sampled air</b>	<b>16</b>
<b>12 Performance characteristics</b>	<b>17</b>
<b>13 Test report</b>	<b>18</b>
<b>14 Quality control</b>	<b>19</b>
<b>Annex A (informative) Total volatile organic compounds (TVOC) and total semi-volatile organic compounds (TSVOC)</b>	<b>20</b>
<b>Annex B (informative) Examples of compounds detected in indoor air and from building products in test chambers</b>	<b>22</b>
<b>Annex C (informative) Description of sorbents</b>	<b>27</b>
<b>Annex D (informative) Guide on sorbent usage</b>	<b>28</b>
<b>Annex E (informative) Safe sampling volumes for selected organic vapours</b>	<b>30</b>
<b>Annex F (informative) Storage recovery of solvents on sorbent tubes</b>	<b>33</b>
<b>Bibliography</b>	<b>35</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

This document was prepared by Technical Committee ISO/TC 146, *Air quality*, Subcommittee SC 6, *Indoor air*.

This third edition cancels and replaces the second edition (ISO 16000-6:2011), which has been technically revised. The main changes compared to the previous edition are as follows:

- other sorbents than Tenax TA® are allowed to be used;
- descriptions of VVOC and SVOC measurements are included in the mandatory part of the document.

A list of all parts in the ISO 16000 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at [www.iso.org/members.html](http://www.iso.org/members.html).


## Introduction

ISO 16000-1 establishes general requirements relating to the measurement of indoor air pollutants and the important conditions to be observed before or during the sampling of individual pollutants or groups of pollutants. Aspects of the determination (sampling and analysis) and the sampling strategy of specific pollutants or groups of pollutants are specified in the subsequent parts of ISO 16000 (see Foreword).

ISO 16000-5 (dealing with VOC sampling strategy) is a link between ISO 16000-1 (a generic standard establishing the principles) and this part of ISO 16000, which deals with sampling and analytical measurements.

ISO 16017 (see [Clause 2](#) and Reference [8]) and ISO 12219 [3]-[7] also focus on measuring vapour-phase organic chemicals in air.

This document can be applied to measure vapour phase organic compounds in indoor environments that include buildings with varying designs and purposes and cabins for different modes of transport, as well as measurement in product emission test chambers. These measurements can be for a range of purposes as described in ISO 16000-1 and ISO 16000-5, therefore the requirement for the measurement may be well defined by the task descriptor or may be quite open. For example, the task may be to determine a specific list of target chemicals with a defined sampling time and sensitivity of measurement or it may be to investigate the cause of a reported and poorly understood indoor air quality problem. Depending upon the task of measurement the user of this document should select the most appropriate sampling and analytical instrumentation and conditions. This document provides that information in the normative part combined with informative guidance. [Figure 1](#) refers to the most critical parts of the standard with regard to selection of the most appropriate methodology for the task to be undertaken. Tenax TA<sup>®1</sup> only or multisorbents can be used to capture ranges of vapour phase organic compounds. Multisorbents are used for wider ranges and may improve recovery of compounds.

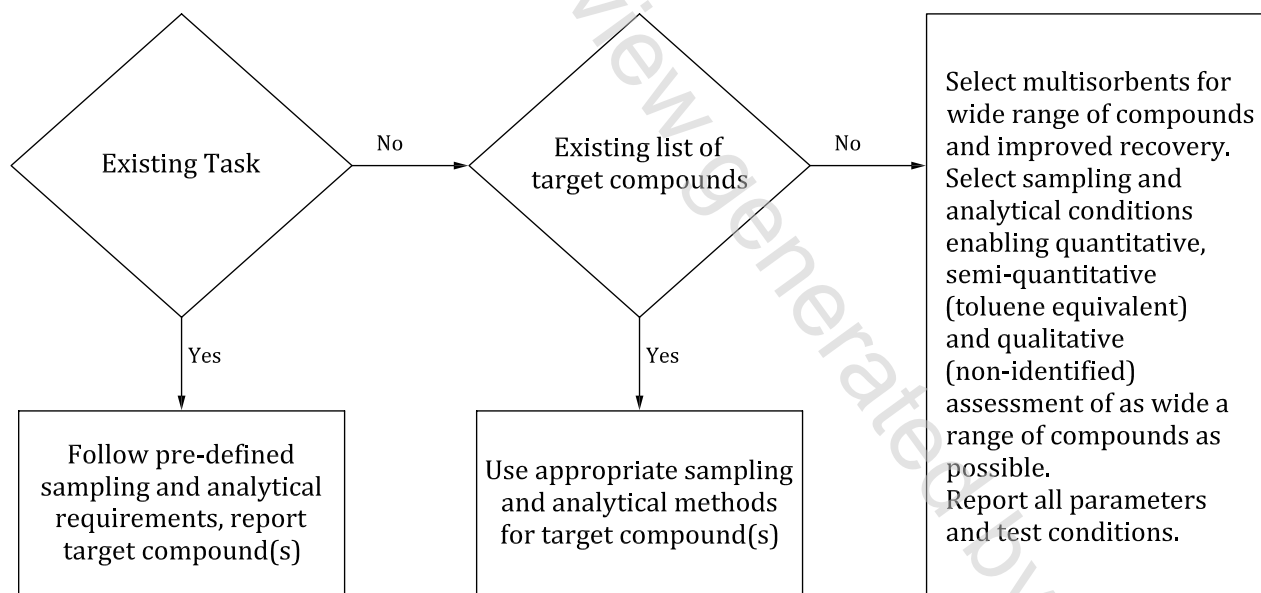

**Figure 1 — Measurement scheme showing different ways of analysing air samples depending on the respective task including target compounds**

1) Tenax TA<sup>®</sup> is a trade name of a product supplied by Buchem. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of the product named. Equivalent products may be used, if they can be shown to lead to the same results.



## Indoor air —

### Part 6:

## Determination of organic compounds (VVOC, VOC, SVOC) in indoor and test chamber air by active sampling on sorbent tubes, thermal desorption and gas chromatography using MS or MS FID

### 1 Scope

This document specifies a method for determination of volatile organic compounds (VOC) in indoor air and in air sampled for the determination of the emission from products or materials used in indoor environments (according to ISO 16000-1) using test chambers and test cells. The method uses sorbent sampling tubes with subsequent thermal desorption (TD) and gas chromatographic (GC) analysis employing a capillary column and a mass spectrometric (MS) detector with or without an additional flame ionisation detector (FID)<sup>[13]</sup>.

The method is applicable to the measurement of most GC-compatible vapour-phase organic compounds at concentrations ranging from micrograms per cubic metre to several milligrams per cubic metre. Many very volatile organic compounds (VVOC) and semi-volatile organic compounds (SVOC) can be analysed depending on the sorbents used.

### 2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 16000-1, *Indoor air — Part 1: General aspects of sampling strategy*

EN 13137, *Workplace atmospheres – Pumps for personal sampling of chemical and biological agents – Requirements and test methods*

### 3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org/>

#### 3.1

##### **semi-volatile organic compound SVOC**

organic compound eluting after n-hexadecane on a gas chromatographic column specified as a 5 % phenyl 95 % methyl polysiloxane phase capillary gas chromatographic column

Note 1 to entry: The vapour-fraction of SVOC ranging in volatility to n-C<sub>44</sub> can also be analysed by thermal desorption GC-MS but requires specific sampling and analytical conditions for optimum performance <sup>[22,25]</sup>.