

This document is a preview generated by EVS

VEE KVALITEET
Analüütiliste meetodite kalibreerimine ja hindamine
ning jõudluskarakteristikute hindamine
Osa 1: Lineaarse kalibreerimisfunktsiooni statistiline
hindamine

Water quality

Calibration and evaluation of analytical methods and
estimation of performance characteristics

Part 1: Statistical evaluation of the linear calibration
function

EESTI STANDARDI EESSÕNA**NATIONAL FOREWORD**

<p>Käesolev Eesti standard EVS-ISO 8466-1:2004 "Vee kvaliteet. Analüütiliste meetodite kalibreerimine ja hindamine ning jõndluskarakteristikute hindamine. Osa 1: Lineaarse kalibreerimisfunktsiooni statistiline hindamine" sisaldb rahvusvahelise standardi ISO 8466-1:1990 "Water quality - Calibration and evaluation of analytical methods and estimation of performance characteristics - Part 1: Statistical evaluation of the linear calibration function" identset ingliskeelsel teksti.</p> <p>Standard EVS-ISO 8466-1:2004 on kinnitatud Eesti Standardikeskuse 19.06.2009 käskkirjaga ja jõustub sellekohase teate avaldamisel EVS Teatajas.</p> <p>Standard on kätesaadav Eesti Standardikeskusest.</p>	<p>This Estonian Standard EVS-ISO 8466-1:2004 consists of the identical English text of the International Standard ISO 8466-1:1990 "Water quality - Calibration and evaluation of analytical methods and estimation of performance characteristics - Part 1: Statistical evaluation of the linear calibration function".</p> <p>This standard is ratified with the order of Estonian Centre for Standardisation dated 19.06.2009 and is endorsed with the notification published in the official bulletin of the Estonian national standardisation organisation.</p> <p>The standard is available from Estonian Centre for Standardisation.</p>
--	---

Käsitlusala	Scope
<p>Kirjeldab samme selle funktsiooni statistiliste karakteristikute hindamiseks. See on rakendatav kalibreerimist vajavate meetodite puhul. Selleks, et tuletada võrreldavaid analüütilisi tulemusi ja et oleks alus analüütilele kvaliteedikontrollile, tuleb kalibreerida ja hinnata samaaegselt. See ISO 8466 osa kirjeldab samme lineaarse kalibreerimisfunktsiooni statistiliste karakteristikute hindamiseks. See on rakendatav kalibreerimist vajavate meetodite puhul. Selle rahvusvahelise standardi edasised osad katavad tuvastuspiiri määramise ja tuvastuspiiri, interferentside mõju ja teised jõndluskarakteristikud.</p> <p>See on mõeldud ainult puhta analüütilise meetodi hindamiseks ja kalibreerimisfunktsiooni jõndluskarakteristikute arvutamiseks.</p> <p>Selleks, et tuletada võrreldavaid analüütilisi tulemusi ja et oleks alus analüütilele kvaliteedikontrollile, tuleb analüütilisi meetodeid kalibreerida ja hinnata samaaegselt.</p>	<p>Describes the steps to be taken in evaluating the statistical characteristics of this function. It is applicable to methods requiring a calibration. In order to derive comparable analytical results and as a basis for analytical quality control the calibration and evaluation have to be performed uniformly. This part of ISO 8466 describes the steps to be taken in evaluating the statistical characteristics of the linear calibration function. It is applicable to methods requiring a calibration. Further parts of this International Standard will cover the determination of limit of detection and limit of determination, the effect of interferences and other performance characteristics.</p> <p>It is intended especially for the evaluation of the pure analytical method and for the calculation of performance characteristics of the calibration function.</p> <p>In order to derive comparable analytical results and as a basis for analytical quality control the calibration and evaluation of analytical methods have to be performed uniformly.</p>

This document is a preview generated by EVS

ICS 13.060.01 Vee kvaliteet üldiselt
Võtmesõnad: hindamine, kalibreerimine, kvaliteedikontroll, kvaliteet, vesi

Standardite reproduutseerimis- ja levitamisõigus kuulub Eesti Standardikeskusele
Andmete paljundamine, taastekitamine, kopeerimine, salvestamine elektroonilisse süsteemi või edastamine üksik millises vormis või millisel teel on keelatud ilma Eesti Standardikeskuse poolt antud kirjaliku loata.
Kui Teil on küsimusi standardite autorikaitse kohta, palun võtke ühendust Eesti Standardikeskusega:
Aru 10 Tallinn 10317 Eesti; www.evs.ee; Telefon: 605 5050; E-post: info@evs.ee

Right to reproduce and distribute belongs to the Estonian Centre for Standardisation
No part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying, without permission in writing from Estonian Centre for Standardisation.
If you have any questions about standards copyright, please contact Estonian Centre for Standardisation:
Aru str 10 Tallinn 10317 Estonia; www.evs.ee; Phone: 605 5050; E-mail: info@evs.ee

This document is a preview generated by EVS

Contents

	Page
Foreword	iii
1 Scope	1
2 Definitions	1
3 Symbols	2
4 Performance	3
4.1 Choice of working range.....	3
4.2 Calibration and characteristics of the method	4
4.3 Assessment	5
5 Example	6
5.1 Choice of working range.....	6
5.2 Calibration and characteristics of the method	7
5.3 Evaluation	7
Annex A Bibliography	8

© ISO 1990

All rights reserved. No part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Organization for Standardization
Case postale 56 • CH-1211 Genève 20 • Switzerland

Printed in Switzerland

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for approval before their acceptance as International Standards by the ISO Council. They are approved in accordance with ISO procedures requiring at least 75 % approval by the member bodies voting.

International Standard ISO 8466-1 was prepared by Technical Committee ISO/TC 147, *Water quality*.

ISO 8466 consists of the following parts, under the general title *Water quality — Calibration and evaluation of analytical methods and estimation of performance characteristics*:

- *Part 1: Statistical evaluation of the linear calibration function*
- *Part 2: Calibration strategy for non-linear calibration functions*
- *Part 3: Method of standard addition*
- *Part 4: Estimation of limit of detection and limit of determination of an analytical basis method.*

Annex A of this part ISO 8466 is for information only.

Water quality – Calibration and evaluation of analytical methods and estimation of performance characteristics

Part 1: Statistical evaluation of the linear calibration function

1 Scope

This part of ISO 8466 describes the steps to be taken in evaluating the statistical characteristics of the linear calibration function. It is applicable to methods requiring a calibration. Further parts of this International Standard will cover the determination of limit of detection and limit of determination, the effect of interferences and other performance characteristics.

It is intended especially for the evaluation of the pure analytical method and for the calculation of performance characteristics of the calibration function.

In order to derive comparable analytical results and as a basis for analytical quality control the calibration and evaluation of analytical methods have to be performed uniformly.

2 Definitions

For the purposes of this part of ISO 8466, the following definitions apply.

2.1 analytical method: An analytical method is composed of procedural, measuring, calibrating and evaluating instructions (see figure 1).

Whereas the procedural and measuring instructions depend on the method, and are therefore the object of standardization of the respective method, the calibrating and evaluating instructions are valid for any analytical method requiring calibration.

2.2 calibrating instruction: Describes the approach to determine the calibration function from information values, y_i , obtained by measuring given standard concentrations, x_i . The slope of the calibration function, b , as a measure of sensitivity of the analytical method and the standard deviation of the method, s_{x_0} , are figures of merit and characteristics which result from the calibration experiment.

The standard deviation, s_{x_0} , allows the comparison of independent analytical methods.

For the user of the method, these characteristics present criteria for the internal laboratory quality control.

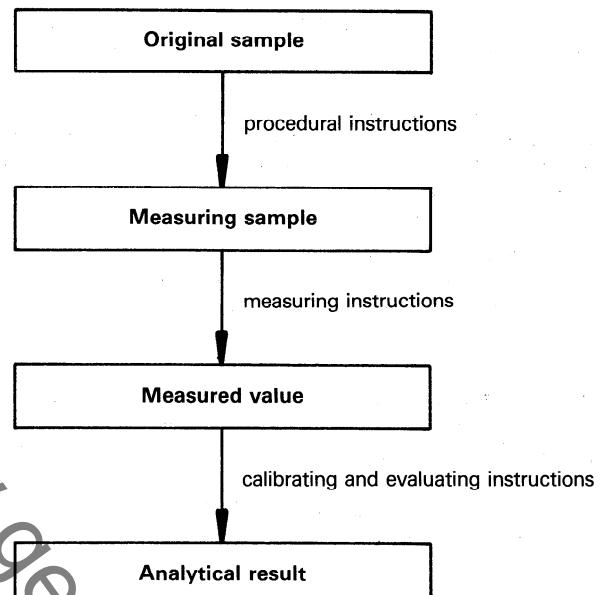


Figure 1 — The analytical method

2.3 evaluating instruction: A calculation guide for the computation of concentrations from the measured values by the use of the calibration function. Additionally, the confidence range permits an objective assessment of the imprecision of the analytical result^[2].

2.4 measured values: The concentration-dependent initial values (e.g. extinction) of a measuring system.

NOTE — Information value and measured volume are synonymous.

2.5 residual standard deviation, s_y : The residual standard deviation describes the scatter of the information values about the calculated regression line. It is a figure of merit, describing the precision of the calibration.

For the purpose of this standard, the standard deviation of the method means the standard of deviation of the calibration procedure.