

This document is a preview generated by EVS

Gas meters - Conversion devices - Part 3: Flow computer

EESTI STANDARDI EESSÕNA

NATIONAL FOREWORD

See Eesti standard EVS-EN 12405-3:2015 sisaldab Euroopa standardi EN 12405-3:2015 ingliskeelset teksti.	This Estonian standard EVS-EN 12405-3:2015 consists of the English text of the European standard EN 12405-3:2015.
Standard on jõustunud sellekohase teate avaldamisega EVS Teatajas	This standard has been endorsed with a notification published in the official bulletin of the Estonian Centre for Standardisation.
Euroopa standardimisorganisatsioonid on teinud Euroopa standardi rahvuslikele liikmetele kättesaadavaks 02.12.2015.	Date of Availability of the European standard is 02.12.2015.
Standard on kättesaadav Eesti Standardikeskusest.	The standard is available from the Estonian Centre for Standardisation.

Tagasisidet standardi sisu kohta on võimalik edastada, kasutades EVS-i veebilehel asuvat tagasiside vormi või saates e-kirja meiliaadressile standardiosakond@evs.ee.

ICS 91.140.40

Standardite reprodutseerimise ja levitamise õigus kuulub Eesti Standardikeskusele

Andmete paljundamine, taastekitamine, kopeerimine, salvestamine elektroonsesse süsteemi või edastamine ükskõik millises vormis või millisel teel ilma Eesti Standardikeskuse kirjaliku loata on keelatud.

Kui Teil on küsimusi standardite autorikaitse kohta, võtke palun ühendust Eesti Standardikeskusega:

Aru 10, 10317 Tallinn, Eesti; koduleht www.evs.ee; telefon 605 5050; e-post info@evs.ee

The right to reproduce and distribute standards belongs to the Estonian Centre for Standardisation

No part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying, without a written permission from the Estonian Centre for Standardisation.

If you have any questions about copyright, please contact Estonian Centre for Standardisation:

Aru 10, 10317 Tallinn, Estonia; homepage www.evs.ee; phone +372 605 5050; e-mail info@evs.ee

English Version

Gas meters - Conversion devices - Part 3: Flow computer

Compteurs de gaz - Dispositifs de conversion - Partie 3:
Calculateurs de débit

Gaszähler - Umwerter - Teil 3: Flowcomputer

This European Standard was approved by CEN on 19 September 2015.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN-CENELEC Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN-CENELEC Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

CEN-CENELEC Management Centre: Avenue Marnix 17, B-1000 Brussels

Contents

Page

European foreword.....	5
Introduction	6
1 Scope	8
2 Normative references	8
3 Terms, definitions and symbols.....	10
3.1 Terms and definitions	10
3.2 Symbols and subscripts	16
3.3 Abbreviations	18
3.4 Environmental classification for flow computers	18
3.4.1 Climatic conditions	18
3.4.2 Mechanical conditions.....	18
3.4.3 Electrical and Electromagnetic conditions	18
4 Principle of measurement	18
4.1 General.....	18
4.2 Correction functions	19
4.2.1 General.....	19
4.2.2 Correction of the volume at measurement conditions.....	20
4.2.3 Temperature and pressure correction of USM body dimension.....	23
4.2.4 Temperature and pressure measurement correction for conversion	23
5 Rated operating conditions	23
5.1 Specified field of measurement.....	23
5.1.1 General.....	23
5.1.2 Specified measurement range for gas pressure.....	23
5.1.3 Specified measurement range for gas temperature	24
5.1.4 Gas characteristics.....	24
5.1.5 Base conditions.....	24
5.2 Environmental conditions	24
5.2.1 Ambient temperature range	24
5.2.2 Humidity range	24
5.3 Power supply	24
6 Construction requirements.....	25
6.1 General.....	25
6.2 Sealing.....	25
6.3 Time measuring functions.....	27
6.3.1 Clock.....	27
6.3.2 Time interval	27
6.4 Casings	28
6.5 Indications	28
6.5.1 General.....	28
6.5.2 Electronic indicating device	30
6.6 Inputs for volume conversion.....	30
6.7 Alarms in flow computer	31
6.7.1 Detection of defective operation situations	31

6.7.2	Handling of volumes during maintenance	31
6.7.3	Memorization of metrological data.....	31
6.7.4	Handling of alarms	31
6.8	Specific monitoring functions performed by flow computer.....	31
6.8.1	General	31
6.8.2	Turbine Meter health check (Mechanical meter)	33
6.8.3	USM health check (meter integrity check)	34
6.8.4	Gas analysis devices health check	35
6.8.5	p -T transducer health check.....	36
6.8.6	Self check of the Z algorithm.....	36
6.8.7	Volume comparison	36
6.8.8	Gas quality comparison	38
6.9	Cut-off function.....	38
6.10	Long-term data storage	38
6.10.1	General	38
6.10.2	Categories of data to be stored	39
6.10.3	Triggers and methods for storage	39
6.10.4	Clock-time stamps.....	40
6.10.5	Security (physical, electronic and software)	40
6.10.6	Error handling	41
6.10.7	Long term data storage – Security audit.....	41
7	Installation requirements	42
7.1	General	42
7.2	Calculator.....	43
7.3	Temperature transducer	43
7.4	Pressure transducer	43
8	Performance.....	44
8.1	Reference conditions.....	44
8.2	Rated operating conditions.....	44
8.3	Maximum permissible errors.....	44
8.3.1	General	44
8.3.2	Global approach: error of main indication.....	45
8.3.3	Modular approach: specific errors for a FC.....	45
8.4	Conditions of matching the constituent elements of a FC.....	45
8.5	Influence factors	46
8.6	Disturbances.....	46
8.7	Durability.....	46
8.8	Repeatability	46
8.9	Reliability	46
8.10	Adjustment and calibration of the transducers.....	47
9	Tests of conformity	47
9.1	Verification of the construction requirements.....	47
9.2	Verification of the performance requirements	48
9.2.1	Test conditions	48
9.2.2	Samples of FC required for testing	49
10	Marking	50
11	Installation and operating instructions	51
Annex A	(normative) Type test.....	52
A.1	General conditions	52
A.2	Accuracy tests under reference conditions.....	54

A.3	Effect of ambient temperature	55
A.4	Effect of damp heat, steady-state test	55
A.5	Effect of damp heat, cyclic test.....	56
A.6	Electrical power variation	56
A.7	Short time power reductions	57
A.8	Electrical bursts	58
A.9	Electromagnetic susceptibility.....	58
A.10	Electrostatic discharges.....	59
A.11	Overload of pressure (only for pressure transducers)	59
A.12	Effect of vibrations.....	60
A.13	Effect of shocks.....	60
A.14	Overload of pressure (mechanical) (only for pressure transducer)	61
A.15	Durability	61
A.16	Alarms operation	62
A.17	Repeatability.....	63
A.18	Short time DC power variations.....	63
A.19	Surges on supply lines and/or signal lines	64
A.20	Power frequency magnetic field	64
Annex B	(normative) Pressure transducers.....	65
B.1	Scope	65
B.2	Rated operating conditions	65
B.3	Construction requirements	65
B.4	Performances	66
B.5	Tests of conformity.....	67
B.6	Marking.....	67
Annex C	(normative) Temperature transducers	68
C.1	Scope	68
C.2	Rated operating conditions	68
C.3	Construction requirements	68
C.4	Performances	69
C.5	Tests of conformity.....	70
C.6	Marking.....	70
Annex D	(normative) Requirements and testing of meter error correction	71
D.1	General.....	71
D.2	Verification of the volumetric flow rate determination.....	71
D.3	Verification of the gas density calculation procedure	71
D.4	Verification of the gas viscosity calculation procedures	72
D.5	Verification of the error transposition from $e(Q_i)$ to $e(Re_i)$	72
D.6	Verification of the error function $\delta(Q)$ or $\delta(Re)$ interpolation or approximation.....	73
D.7	Verification of correction factor $F(Q)$ or $F(Re)$, corrected flow rate and corrected volume determination.....	73
D.8	Verification of the activation and deactivation of error correction calculations on limits of its application.....	73
Annex E	(informative) Range of application of meter error correction with functions: $e(Q)$ or $e(Re)$	74
E.1	General.....	74
E.2	Range of application.....	74
E.3	Example for turbine meters working at p_{op} nearly constant.....	75
Bibliography		77

European foreword

This document (EN 12405-3:2015) has been prepared by Technical Committee CEN/TC 237 “Gas meters”, the secretariat of which is held by BSI.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by June 2016, and conflicting national standards shall be withdrawn at the latest by June 2016.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

EN 12405 consists of the following parts:

- Part 1: Volume conversion (and its amendments EN 12405-1:2005/A1:2006 and EN 12405-1:2005+A2:2010 to allow the harmonization of the standard with the Measuring Instruments Directive 2004/22/EC);
- Part 2: Energy conversion;
- Part 3: flow computer (this European Standard).

In the preparation of this European Standard, the content of OIML Publication, “Recommendation 140 – measuring systems for gaseous fuel”, has been taken into account.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and the United Kingdom.

Introduction

A high accuracy volume conversion device can be needed depending of the intended use. EN 12405-3 is established in order to meet severe requirements concerning accuracy and related functions.

For the purpose of this European Standard, functions are described, although these functions can be physically located in different components (e.g. calibration curve programmed in the measuring equipment itself or in the calculator).

Four main categories of functions are described to achieve data processing:

- Sensor signal Acquisition functions: to process signals from physical quantity provided by sensors and transducers to measurands;
- Sensor functions: to convert measurands to correct measurements, mostly based upon calibration results and filtering procedures;
- Metering functions: to calculate derived values such as volume, calorific value, compression factor etc. based upon international standards and formulas and to take care of the supervision and monitoring for the purpose of high accuracy and substitution values;
- Long Term Data Storage functions: to keep all relevant information necessary to construct or reconstruct calculated values:
 - for later legally relevant purposes (e.g. the conclusion of a commercial transaction);
 - for back up of the relevant data.

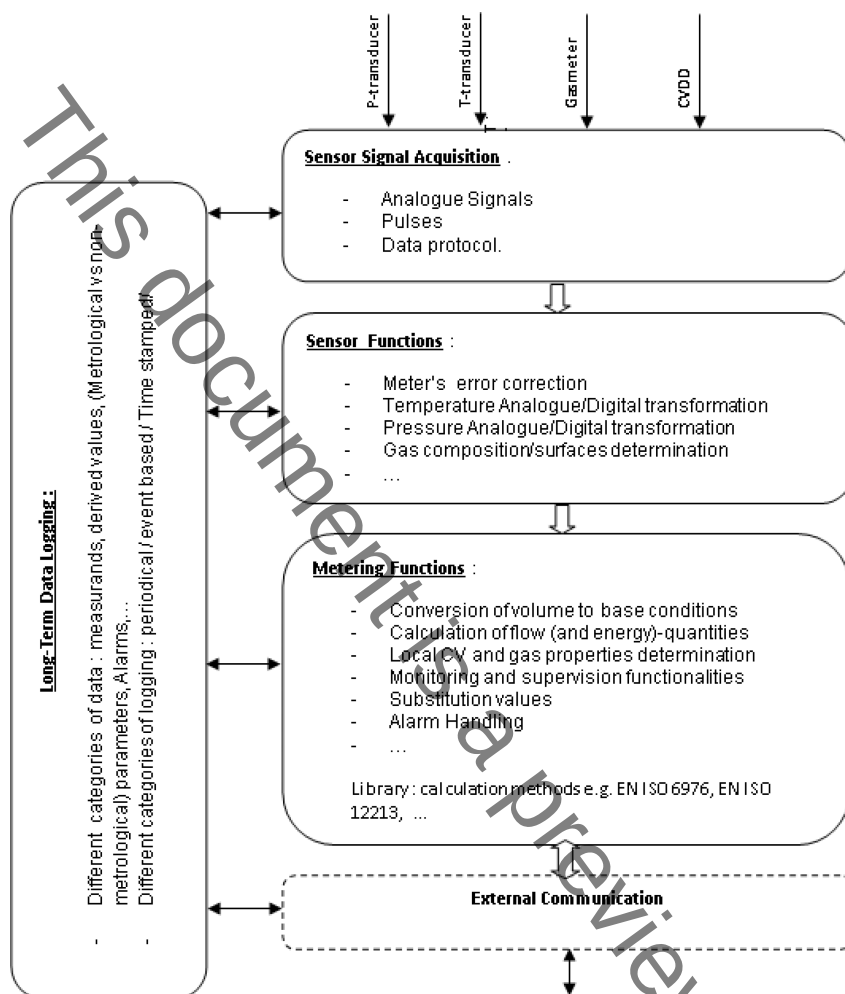


Figure 1 — Description of the functionalities of the flow computer calculator

Modular and global approaches

In the modular approach, the flow computer is an assembly of separate associated measuring instruments and a calculator, which are verified separately. Each instrument is verified according to its testing procedure, using the indication available on the calculator or on the associated measuring instrument itself. In this case, the indication shall correspond to the indication of that measuring instrument, which is directly performing volume conversion. The verification of the functions consists in verifying the calculation concerning each characteristic quantity of the gas and/or the calculation for the volume conversion.

In case of external communication, sufficient resolution of required data is ensured during data transmission.

The associated measuring instruments are validated for or with a type calculator in order to ensure the interoperability of the association.

CVDD is covered in EN 12405-2.

In the global approach, the flow computer is tested as a package including the calculator and its associated measuring instruments and functions.

The testing procedures are given in Annex A.

1 Scope

Part 3 of this European Standard specifies the requirements and tests for the construction, performance, safety and conformity of flow computers (FCs) used to meet the metrological and technical requirements of a high accuracy volume conversion device.

They are used to determine volume of fuel gases, including those of the first and second families according to EN 437.

For the purpose of this European Standard, only flow computers that are intended to operate with ultrasonic meters according to ISO 17089-1 or gas turbine meters conforming to EN 12261 are considered.

For the purpose of this European Standard only classification classes E2 and M1 are considered for the flow computer calculator.

FCs are equipped with external separate transducers for pressure and temperature which may be approved separately.

The provisions concerning pressure and temperature transducers are given in Annex B and C.

Requirements and tests are given for energy calculator in EN 12405-2.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

EN 437, *Test gases — Test pressures — Appliance categories*

EN 1776, *Gas supply systems — Natural gas measuring stations — Functional requirements*

EN 12261, *Gas meters — Turbine gas meters*

EN 12405-1:2005+A2:2010, *Gas meters — Conversion devices — Part 1: Volume conversion*

EN 12405-2, *Gas meters — Conversion devices — Part 2: Energy conversion*

EN 55011, *Industrial, scientific and medical equipment — Radio-frequency disturbance characteristics — Limits and methods of measurement (CISPR 11, modified)*

EN 60068-2-1, *Environmental testing — Part 2-1: Tests — Test A: Cold (IEC 60068-2-1)*

EN 60068-2-2, *Environmental testing — Part 2-2: Tests — Test B: Dry heat (IEC 60068-2-2)*

EN 60068-2-30, *Environmental testing — Part 2-30: Tests — Test Db: Damp heat, cyclic (12 h + 12 h cycle) (IEC 60068-2-30)*

EN 60068-2-31, *Environmental testing — Part 2-31: Tests — Test Ec: Rough handling shocks, primarily for equipment-type specimens (IEC 60068-2-31)*

EN 60068-2-64, *Environmental testing — Part 2-64: Tests — Test Fh: Vibration, broadband random and guidance (IEC 60068-2-64)*

EN 60068-2-78, *Environmental testing — Part 2-78: Tests — Test Cab: Damp heat, steady state (IEC 60068-2-78)*

- EN 60068-3-1, *Environmental testing — Part 3-1: Supporting documentation and guidance — Cold and dry heat tests (IEC 60068-3-1)*
- EN 60079-0, *Explosive atmospheres — Part 0: Equipment — General requirements (IEC 60079-0)*
- EN 60079-7, *Explosive atmospheres — Part 7: Equipment protection by increased safety "e" (IEC 60079-7)*
- EN 60079-11, *Explosive atmospheres — Part 11: Equipment protection by intrinsic safety "i" (IEC 60079-11)*
- EN 60079-25, *Explosive atmospheres — Part 25: Intrinsically safe electrical systems (IEC 60079-25)*
- EN 60529, *Degrees of protection provided by enclosures (IP Code) (IEC 60529)*
- EN 60751, *Industrial platinum resistance thermometers and platinum temperature sensors (IEC 60751)*
- EN 60947-5-6, *Low-voltage switchgear and controlgear — Part 5-6: Control circuit devices and switching elements — DC interface for proximity sensors and switching amplifiers (NAMUR) (IEC 60947-5-6)*
- EN 60950-1, *Information technology equipment — Safety — Part 1: General requirements (IEC 60950-1)*
- EN 61000-4-1, *Electromagnetic compatibility (EMC) — Part 4-1: Testing and measurement techniques — Overview of IEC 61000-4 series (IEC 61000-4-1)*
- EN 61000-4-2, *Electromagnetic compatibility (EMC) — Part 4-2: Testing and measurement techniques — Electrostatic discharge immunity test (IEC 61000-4-2)*
- EN 61000-4-3, *Electromagnetic compatibility (EMC) — Part 4-3: Testing and measurement techniques — Radiated, radio-frequency, electromagnetic field immunity test (IEC 61000-4-3)*
- EN 61000-4-4, *Electromagnetic compatibility (EMC) — Part 4-4: Testing and measurement techniques — Electrical fast transient/burst immunity test (IEC 61000-4-4)*
- EN 61000-4-5, *Electromagnetic compatibility (EMC) — Part 4-5: Testing and measurement techniques — Surge immunity test (IEC 61000-4-5)*
- EN 61000-4-6, *Electromagnetic compatibility (EMC) — Part 4-6: Testing and measurement techniques — Section 6: Immunity to conducted disturbances, induced by radio-frequency fields (IEC 61000-4-6)*
- EN 61000-4-8, *Electromagnetic compatibility (EMC) — Part 4-8: Testing and measurement techniques — Power frequency magnetic field immunity test (IEC 61000-4-8)*
- EN 61000-4-11, *Electromagnetic compatibility (EMC) — Part 4-11: Testing and measurement techniques — Voltage dips, short interruptions and voltage variations immunity tests (IEC 61000-4-11)*
- EN 61000-4-29, *Electromagnetic compatibility (EMC) — Part 4-29: Testing and measurement techniques — Voltage dips, short interruptions and voltage variations on d.c. input power port immunity tests (IEC 61000-4-29)*
- EN 62054-21, *Electricity metering (a.c.) — Tariff and load control — Part 21: Particular requirements for time switches (IEC 62054-21)*
- EN 62262, *Degrees of protection provided by enclosures for electrical equipment against external mechanical impacts (IK code) (IEC 62262)*

EN ISO 6976, *Natural gas — Calculation of calorific values, density, relative density and Wobbe index from composition (ISO 6976)*

EN ISO 12213-2:2009, *Natural gas — Calculation of compression factor — Part 2: Calculation using molar-composition analysis (ISO 12213-2:2006)*

EN ISO 12213-3:2009, *Natural gas — Calculation of compression factor — Part 3: Calculation using physical properties (ISO 12213-3:2006)*

EN ISO 15970, *Natural gas — Measurement of properties — Volumetric properties: density, pressure, temperature and compression factor (ISO 15970)*

IEC 61520, *Metal thermowells for thermometer sensors — Functional dimensions*

ISO 17089-1, *Measurement of fluid flow in closed conduits — Ultrasonic meters for gas — Part 1: Meters for custody transfer and allocation measurement*

ISO/IEC/IEEE 60559, *Information technology — Microprocessor Systems — Floating-Point arithmetic*

3 Terms, definitions and symbols

3.1 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1.1

absolute pressure

value of the pressure of the gas relative to vacuum

3.1.2

associated measuring instrument

instrument for measuring certain quantities which are characteristic of the gas, e.g. temperature, pressure, or calorific value, whose indications are used by the calculator with a view to making a correction and/or a conversion

Note 1 to entry: For the purpose of this European Standard, when dealing with the ECD in modular approach, the VCD and CVDD are considered as associated measuring instrument.

3.1.3

base conditions

fixed conditions used to express the volume of gas independently of the measurement conditions and the superior calorific value

Note 1 to entry: The pressure base for both volumetric metering and combustion is always 1,01325 bar. The temperature is specified.

EXAMPLE Temperature of 273,15 K and absolute pressure of 1,013 25 bar or temperature of 288,15 K and absolute pressure of 1,013 25 bar.

3.1.4

calculator

electronic device that receives the output signals from measuring and data acquisition systems, e.g. associated gas meter or transducers, and processes them