Pöörlevad hambaraviinstrumendid. Freesid. Osa 3: Laboris kasutatavad freespinkide jaoks mõeldud karbiidfreesid

Dental rotary instruments - Cutters - Part 3: Carbide laboratory cutters for milling machines



EESTI STANDARDI EESSÕNA

NATIONAL FOREWORD

Käesolev Eesti standard EVS-EN 27787-3:1999 sisaldab Euroopa standardi EN 27787-3:1993 ingliskeelset teksti. Standard on kinnitatud Eesti Standardikeskuse 12.12.1999 käskkirjaga ja jõustub sellekohase teate avaldamisel EVS Teatajas.	This Estonian standard EVS-EN 27787-3:1999 consists of the English text of the European standard EN 27787-3:1993. This standard is ratified with the order of Estonian Centre for Standardisation dated 12.12.1999 and is endorsed with the notification published in the official bulletin of the Estonian national standardisation organisation.
Standard on kättesaadav testi standardiorganisatsioonist.	The standard is available from Estonian standardisation organisation.
ICS 11.060.20	The standard is available from Estonian standardisation organisation.
Andmete paljundamine, taastekitamine, kopeerimine, salvestamine e millisel teel on keelatud ilma Eesti Standardikeskuse poolt antud kirja	
Kui Teil on küsimusi standardite autorikaitse kohta, palun võtke ühen Aru 10 Tallinn 10317 Eesti; <u>www.evs.ee;</u> Telefon: 605 5050; E-pos	idust Eesti Standardikeskusega:

Right to reproduce and distribute Estonian Standards belongs to the Estonian Centre for Standardisation

No part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying, without permission in writing from Estonian Centre for Standardisation.

If you have any questions about standards copyright, please contact Estonian Centre for Standardisation: Aru str 10 Tallinn 10317 Estonia; www.evs.ee; Phone: +372 605 5050; E-mail: info@evs.ee

EUROPEAN STANDARD

EN 27787-3

NORME EUROPÉENNE


EUROPÄISCHE NORM

December 1993

UDC 616.314-72:621.914.2

Descriptors:

Dentistry, laboratory equipment, dental rotary-cutting instruments, milling cutters, specifications, dimensions, dimensional tolerances

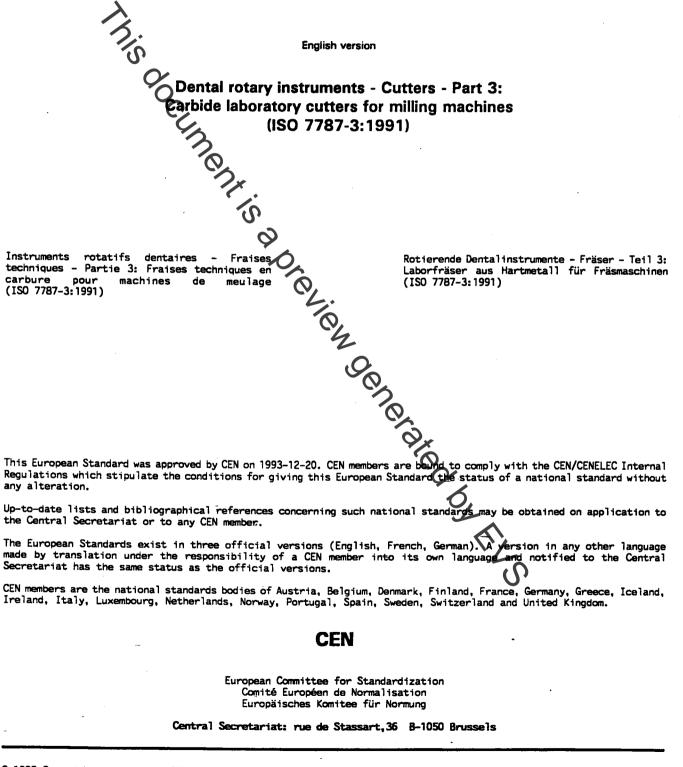

• 1993 Copyright reserved to CEN members

Page 2 EN 27787-3:1993

Foreword

This European Standard has been taken over by Technical Committee CEN/TC 55 "Dentistry" from the work of ISO/TC 106 "Dentistry" of the International Standardization Organization (ISO).

The text was submitted to the Unique Acceptance Procedure (UAP) and approved as a European Standard.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by June 1994, and conflicting national standards shall be withdrawn at the latest by June 1994.

In accordance with the CEN/CENELEC Internal Regulations, following countries are bound to implement this European Standard, Austria, Belgium, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and United Kingdom.

Endorsement notice

The text of the international standard ISO 778731991 was approved by CEN as a European Standard without any modification.

NOTE: Normative references to international publications are listed in annex ZA (normative).

Annex ZA (normative) Normative references to international publications with their relevant European publications


This European Standard incorporates by dated or undated reference, provisions from other publications. These normative references are cited at the appropriate places in the text and the publications are listed hereafter. For dated references, subsequent amendments to or revisions of any of these publications apply to this European Standard only when incorporated in it by amendment or revision. For undated references the latest edition of the publication referred to applies (including amendments).

		Dy Dy		
Publication	<u>Year</u>	Title 0	<u>EN/HD</u>	<u>Year</u>
ISO 1797-1	1991	Dental rotary instruments Shanks - Part 1: Shanks made of metals		
ISO 2157	1984	Dental rotary instruments - Nominal sizes and designation	EN 22157	1989
ISO 2859-1	1989	Sampling procedures for inspection by attributes - Part 1: Sampling plans indexed by acceptable quality level (AQL) for lot-by-lot inspection		-
ISO 6360-1	1985	Dental rotary instruments - Number coding system - Part 1: General characteristics	EN 26360-1	1990
ISO 8325	1985	Dentistry rotary instruments - Test methods	EN 28325	1990
			1 T	

INTERNATIONAL STANDARD

ISO 7787-3

> First edition 1991-12-15

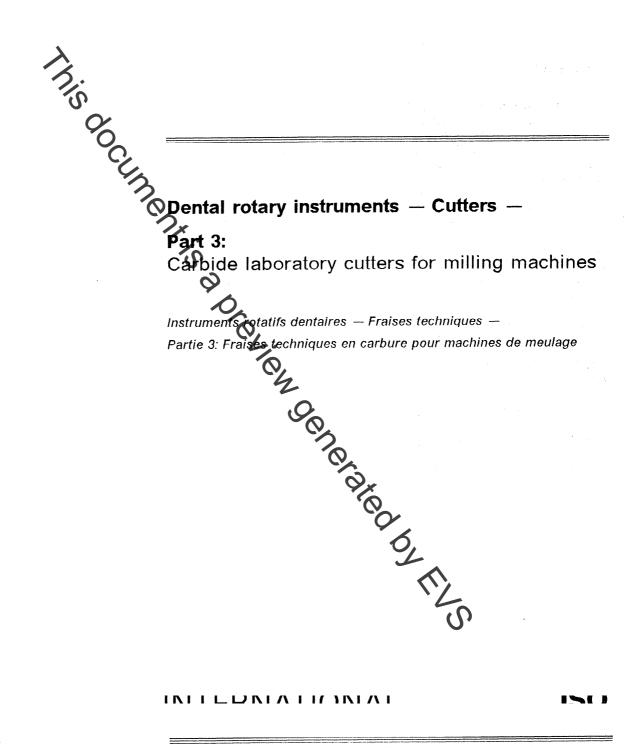



Reference number ISO 7787-3:1991(E)

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each mertiler body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the international Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the Chnical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at lease 75% of the member bodies casting a vote.

International Standard ISO 7787-3 was prepared by Technical Committee ISO/TC 106, Dentistry, Sub-Committee SC 4, Dental instruments.

ISO 7787 consists of the following parts, under the general the Dental Generated by FLS rotary instruments - Cutters:

- Part 1: Steel laboratory cutters
- Part 2: Carbide laboratory cutters
- Part 3: Carbide laboratory cutters for milling machines

© ISO 1991

All rights reserved. No part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Organization for Standardization

Case Postale 56 • CH-1211 Genève 20 • Switzerland

Printed in Switzerland

Dental rotary instruments — Cutters —

Part 3: Carbide laboratory cutters for milling machines

1 Scope

This part of ISO 7787 specifies the dimensional and other requirements for the three most commonly used carbide cutters for milling machines which are predominantly used in the dental laboratory

Special characteristics of cutters, for example spiralled blades, cross-cut, are not covered by this International Standard. These will be dealt with in future International Standard.

Attention is drawn to ISO 6360-1 which specifies a 15 digit number for the identification of dental rotary instruments of all types.

NOTE 1 The various dimensional and other requirements specified for carbide cutters are those considered important to ensure the interchangeability of these instruments.

2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this part of ISO 7787. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this part of ISO 7787 are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 1797-1:1991¹⁾, Dental rotary instruments — Shanks — Part 1: Shanks made of metals.

ISO 2157:1984, Dental rotary instruments — Nominal sizes and designation.

ISO 2859-1:1989, Sampling procedures for inspection by attributes — Part 1: Sampling plans indexed by acceptable quality level (AQL) for lot-by-lot inspection.

ISO 6360-1:1985, Dental rotary instruments — Number coding system — Part 1: General characteristics.

SO 8325:1985, Dental rotary instruments — Test methods.

3 Symbols

The following symbols are used in this part of ISO 7787:

- d_1 diameter of the working part, head diameter
- d_2 diameter at the end of the working part
- l_1 length of the working part, head length
- l_2 overall length of instrument

4 Material

The shaft shall be made of steel or other suitable material.

The working part shall be made of tungsten carbide.

The selection of the type of material and the treatment given to it is left to the discretion of the manufacturer.

¹⁾ To be published.